

# INFUSOVET IP INFUSION PUMP

## USER MANUAL



Item no. 402085

TELEPHONE +49 7461 96 580 0

[www.eickemeyer.com](http://www.eickemeyer.com)

veterinary technology for life  
**Eickemeyer**®





Release date: 202 -0

Revision: .0

---

# Preface

## Manual Purpose

This manual contains the instructions necessary to operate the product safely and in accordance with its function and intended use. Observance of this manual is a prerequisite for proper product performance and correct operation and ensures animal and operator safety.

This manual is based on the maximum configuration and therefore some contents may not apply to your product. If you have any question, please contact us.

This manual is an integral part of the product. It should always be kept close to the equipment so that it can be obtained conveniently when needed.

## Intended Audience

This manual is geared for veterinarians who are expected to have a working knowledge of medical procedures, practices and terminology as required for monitoring of critically ill animals.

## Illustrations

All illustrations in this manual serve as examples only. They may not necessarily reflect the setup or data displayed on your equipment.

## Conventions

- ***Italic text*** is used in this manual to quote the referenced chapters or sections.
- **[ ]** is used to enclose screen texts.
- **<>** is used to enclose the keys.
- **→** is used to indicate operational procedures.

---

# Contents

<b>Preface</b> .....	<b>II</b>
<b>1 Safety</b> .....	<b>1-1</b>
1.1 Safety Information .....	1-1
1.1.1 Dangers.....	1-1
1.1.2 WARNING .....	1-2
1.1.3 CAUTION .....	1-3
1.1.4 NOTE .....	1-4
1.2 Equipment Symbols.....	1-5
<b>2 Overview</b> .....	<b>2-1</b>
2.1 Description .....	2-1
2.1.1 Indications for Use.....	2-1
2.1.2 Contraindications.....	2-1
2.1.3 Appearance, Parts and Features .....	2-1
2.2 Host .....	2-2
2.2.1 Front View .....	2-2
2.2.2 Front View with the Door Opened.....	2-4
2.2.3 Rear View.....	2-5
2.3 Screen Display .....	2-6
2.4 Cursor.....	2-6
<b>3 Installation and Setting</b> .....	<b>3-1</b>
3.1 Installation .....	3-1
3.1.1 Out of Box Audit (OOBA).....	3-2
3.1.2 Operating Conditions.....	3-2
3.1.3 Mount the Clamp .....	3-3
3.1.3.1 Standard Pole Clamp.....	3-3
3.1.3.2 Advanced Pole Clamp (Optional).....	3-4
3.1.4 Connect the AC Power Source .....	3-5
3.1.5 Install and Operate the Drop Sensor (Optional) .....	3-5
3.2 Conventional Settings.....	3-7
3.2.1 Set Language .....	3-7
3.2.2 Adjust Screen Contrast.....	3-7
3.2.3 Set Date and Time.....	3-8
3.2.4 Adjust Volume.....	3-8
3.3 Restore Factory Default.....	3-8
<b>4 Basic Operation</b> .....	<b>4-1</b>
4.1 Infusion Flow Chart.....	4-1

---

4.2 Operational Procedures.....	4-2
4.2.1 Turn on the Pump.....	4-2
4.2.2 Load the Infusion Set .....	4-2
4.2.3 Change the Infusion Set.....	4-4
4.2.4 Change the Infusion Bottle (Bag) .....	4-4
4.2.5 Select Infusion Set Brand .....	4-4
4.2.6 Infusion Mode.....	4-5
4.2.7 Purge.....	4-6
4.2.8 Set Infusion Parameters.....	4-6
4.2.9 Infusion.....	4-6
4.2.10 BOLUS .....	4-7
4.2.11 Change the Rate during Operation .....	4-7
4.2.12 Complete .....	4-8
4.2.13 Standby .....	4-8
4.2.14 Turn off the Pump.....	4-8
<b>5 Setting Parameters .....</b>	<b>5-1</b>
5.1 KVO.....	5-1
5.2 Occlusion Pressure .....	5-1
5.2.1 Set Occlusion Pressure .....	5-1
5.2.2 Set Pressure Unit .....	5-2
5.2.3 Dynamic Pressure Scanning (DPS) .....	5-2
5.2.4 Automatic Pressure Release Function (Anti-Bolus).....	5-2
5.3 Set the Air Bubble Size.....	5-2
5.4 Accumulated Bubble.....	5-3
5.5 Key Lock Function .....	5-3
5.6 Reminder Function .....	5-3
5.7 Time Near End.....	5-4
5.8 Common Infusion Set Brands.....	5-4
5.9 Bed No. Settings.....	5-4
5.10 View Department .....	5-5
5.11 Set the Sensitivity of Empty Bottle Alarm .....	5-5
<b>6 Other Functions .....</b>	<b>6-1</b>
6.1 Nurse Call.....	6-1
6.2 Wireless Networking (Optional) .....	6-2
6.3 Data Export.....	6-3
6.4 WLAN Setting.....	6-3
<b>7 Alarms .....</b>	<b>7-1</b>
7.1 Alarm Level.....	7-1
7.2 Alarm Types.....	7-1
7.2.1 Multi-level Alarm Rules .....	7-2
7.3 Alarm Handling Rules .....	7-2

---

---

7.4 Alarm Countermeasures .....	7-3
<b>8 Battery.....</b>	<b>8-1</b>
8.1 Battery Performance Optimization.....	8-2
8.2 Check the Battery .....	8-2
8.3 Battery Recycling.....	8-3
<b>9 Preservation and Sanitation.....</b>	<b>9-1</b>
9.1 Description .....	9-1
9.2 Cleaning .....	9-1
9.3 Disinfection .....	9-2
<b>10 Maintenance .....</b>	<b>10-1</b>
10.1 Inspection .....	10-1
10.2 Maintenance Plan.....	10-2
10.3 View Information.....	10-2
10.4 Safe Disposal and Recycling .....	10-2
<b>11 Accessories .....</b>	<b>11-1</b>
<b>A Product Specifications.....</b>	<b>A-1</b>
A.1 Safety Specifications.....	A-1
A.1.1 Product Classification.....	A-1
A.1.2 Operating Environment .....	A-2
A.2 Physical Specifications.....	A-2
A.3 Hardware Specifications .....	A-3
A.3.1 Display .....	A-3
A.3.2 Battery.....	A-3
A.3.3 Host LED.....	A-3
A.3.4 Auditory Indicator .....	A-4
A.3.5 External Ports .....	A-4
A.3.6 Signal Output Interface .....	A-4
A.4 Wi-Fi Specifications.....	A-5
A.5 Specifications .....	A-5
A.6 A Reference Table Showing Occlusion Alarm Delay and Possible Dose.....	A-7
A.7 Infusion Accuracy Curve and Trumpet Curve .....	A-8
<b>B EMC and Radio Regulatory Compliance .....</b>	<b>B-1</b>
B.1 EMC .....	B-1
B.2 Radio Regulatory Compliance.....	B-6
<b>C Default Factory Settings .....</b>	<b>C-1</b>
C.1 Alarms.....	C-1
C.2 Interface.....	C-1

---

---

C.3 Parameters .....	C-1
C.4 System Time .....	C-2
<b>D Alarm Information.....</b>	<b>D-1</b>
<b>E Symbols and Terms .....</b>	<b>E-1</b>
E.1 List of Units .....	E-1
E.2 List of Symbols.....	E-2
E.3 List of Terms.....	E-2
E.4 List of Unit Conversion .....	E-4
<b>F Toxic and Hazardous Substances or Elements.....</b>	<b>F-1</b>

# 1 Safety

---

---

## 1.1 Safety Information

The safety statements presented in this chapter refer to basic safety information that the operator must pay attention to and abide by when using the veterinary infusion pump. There are additional safety statements in other chapters or sections, which may be the same as or similar to the following, or specific to particular operations.

---

---

### **Dangers**

---

- Indicates an imminent hazard that, if not avoided, could result in death, serious injury or damage to product/property.
- 
- 

### **WARNING**

---

- Indicates a potential hazard or unsafe practice that, if not avoided, could result in death, serious injury or damage to product/property.
- 
- 

### **CAUTION**

---

- Indicates a potential hazard or unsafe practice that, if not avoided, could result in minor personal injury, product malfunction or damage to product/property.
- 
- 

### **NOTE**

---

- Provides application tips or other useful information to ensure that you get the most out of the product.
- 
- 

### 1.1.1 Dangers

This Manual does not contain any information at the "Danger" level.

---

## 1.1.2 WARNING

---

### WARNING

---

- Device, cables and accessories must be inspected before use to guarantee their normal and safe operation.
  - This equipment can only be connected to the socket with ground protection. Please adopt a rechargeable battery instead of the socket as the power supply if the socket is not provided with a ground lead.
  - To prevent fire or explosion, do not operate the equipment in the presence of anesthetic, flammable or explosive materials.
  - Do not open the equipment casing as there is the impending danger of electric shock. Equipment maintenance and upgrades must be carried out by maintenance technicians whom are trained and licensed by the manufacturer. Moreover, the process must be done only after the AC power supply is disconnected. Maintenance carried out by individuals non-affiliated to the manufacturer or by non-licensed personnel may affect the safety, performance and function of the product.
  - When used with electrosurgery equipment, the safety of animals should be ensured.
  - The animal's condition and the working condition of the veterinary infusion pump must be monitored carefully, the alarm volume and alarm levels need to be set according to the actual needs. Operation and performance relying solely on the auditory alarm system alone is not sufficient, and setting the alarm at a low volume may endanger the animal. If the alarm volume is less than the surroundings volume, which can further lead to operators identify alarm mistakenly.
  - Please carefully install the power line and cables with various accessories to prevent the animal from choking or suffocation caused by entanglement of the cables or by electrical disturbance.
  - The packaging materials must be disposed of in compliance with local laws and regulations or the pet hospital policy on waste management. They must be kept out of the reach of children.
  - Infusion set knots, filter coagulation and occlusions arising from needle insertion can cause the pressure inside the infusion set to rise during infusion. When this occurs, removing the occlusion can cause excessive liquid drug to be infused into the animal, so appropriate measures should be taken.
  - It is recommended that veterinary infusion pump is used with infusion sets recommended by manufacturers (please refer to *5.8 Recommended Infusion Sets List* for specific brands). When use of non-recommended
-

---

---

infusion sets, please make sure to confirm relevant infusion performance (such as accuracy, bubble and pressure) on veterinary infusion pump, and contact the company for calibration service, the infusion sets can only be used after confirmation, otherwise we is not responsible for infusion performance (such as accuracy, bubble and pressure) and relevant alarm function of the veterinary infusion pump.

- Its accuracy cannot be guaranteed when the pump is used with an infusion set without calibration.
  - Do not touch the animal when connecting the peripheral equipment via the input/output signal ports to prevent animal leakage current from exceeding the requirements specified by the standard.
  - In the process of defibrillation, do not touch animal and other non-defibrillation equipments to prevent electric shock damage, and defibrillation will not affect the basic performance (such as infusion accuracy, alarm and signal transmission) of the pump.
- 

### 1.1.3 CAUTION

---

#### CAUTION

---

- Use the accessories specified in this Operator's Manual to guarantee the animal's safety.
  - When this veterinary infusion pump and its accessories exceed their service life, they must be disposed of in accordance with local statutes or pet hospital regulations. If you have any queries, please contact your distributor or the manufacturer.
  - After loading the infusion set and before infusion, check for leakages. If any are found, they should be rectified as soon as possible.
  - For SK series infusion sets, it is recommended to replace the infusion set or adjust the fixing site of the infusion set after the infusion has been running for 36 hours to guarantee accuracy. For infusion sets of other brand, it is recommended to test the service life of the infusion set to determine the time interval of changing the fixing site of the infusion set; if the service life of the infusion set is not tested, it is recommended to adjust the fixing site of the infusion set every 4-8 hours after infusion begins to guarantee accuracy.
  - Electromagnetic fields may affect equipment performance. This makes it necessary for other equipment used in the vicinity of the pump to meet EMC standards. Mobile phones, X ray and MRI equipment are all
-

---

---

potential interference sources because of their high-intensity electromagnetic radiation.

- Before the equipment is connected to the power supply, check that the voltage and frequency of the power supply match the specifications on the label or in this Operator's Manual.
  - Please install and carry the equipment correctly to protect the equipment from damage from drops, impacts, violent shaking or other external mechanical forces.
  - Disposable accessories must be disposed of after use in accordance with the relevant pet hospital regulations.
  - Avoid direct sunshine, high temperatures and dampness.
  - Check the built-in battery before use to make sure it has sufficient power. Recharge the battery if necessary.
  - The infusion set with the luer taper is recommended for use, which can effectively prevent animals from under current caused by the occurrence of the cannula to slip out when under tension.
- 

#### 1.1.4 NOTE

##### NOTE

---

- Install the equipment in a position where it can be easily accessed for inspection, operation and maintenance.
  - Keep this Operator's Manual near to the equipment for future ease of reference.
  - The software of the equipment is developed according to the software development demands of IEC60601-1 standard, which can minimize the possibility of the risk caused by program error.
  - This Operator's Manual describes the most complete functional configuration of the equipment. The product you are using may not have some of the settings or functions described herein.
  - Do not insert devices that are not specified by the manufacturer into the DB9 interfaces.
  - During infusion, the veterinary infusion pump can accurately control the rate, infusion volume and infusion time, and monitor the operation in real-time, to effectively prevent over currents, under currents and instances of backflow.
  - The device is not in touch with the drugs or animals directly. Thus, there is no need to process Biocompatibility test on it.
-

## 1.2 Equipment Symbols

The equipment you purchased may not provide you with all the following symbols.

	Consult instructions for use		ON/OFF
	Alternating current power supply (AC)		Battery
	Alarms		AUDIO PAUSED
	Clear/Back		Start
	Bolus		Confirm
	Stop		Menu
	Move up/Increase		Move down/Decrease
	Move left		Move right
	Infusion set		Caution
	Wireless modules work in order		Wireless transceiver
	DB9 interface		Drop sensor interface
	Lock		Protected against defibrillation CF applied parts
	Date of manufacture		Manufacturer
	This way up		Keep dry
	Fragile, handle with care		Stacking limit by number

<b>IP34</b>	Protected against solid foreign objects with a diameter no less than 2.5mm and protected against spraying liquid water		Environmentally-friendly use periods of electronic products (20 years)
	Temperature limit		CE mark
	Recycle	 801341	NRTL certification mark
	Atmospheric pressure limitation		Humidity limitation
	Serial number	/	/
	The following definition of the WEEE label applies to EU member states only: the use of this symbol indicates that waste electrical and electronic equipment must not be disposed of as unsorted municipal waste and must be collected separately. By ensuring that this product is disposed of correctly, you will help prevent bringing potential negative consequences to the environment and human health. For more detailed information with regard to returning and recycling this product, please consult the distributor from whom you purchased the product		

# 2 Overview

---

---

## 2.1 Description

### 2.1.1 Indications for Use

The veterinary infusion pump is used in conjunction with the infusion set to control the dose of liquid infused into the animal's body.

This veterinary infusion pump is expected to be used in institutes or units with healthcare capabilities.

---

### **WARNING**

---

- **The veterinary infusion pump is for accurate and continuous infusion to animals. It must only be used under appropriate conditions by professional veterinarians or by suitably trained veterinarians. Personnel using this product must receive sufficient training. This product must not be operated by anyone who has not been authorized to do so or has not received suitable training.**
- 

### 2.1.2 Contraindications

None


### 2.1.3 Appearance, Parts and Features

The veterinary infusion pump primarily consists of a housing and built-in battery. Eccentric camshaft is driven by stepper motor during operation, making the fixed upper slider moves up and down sequentially and regularly, infusion set is extruded regularly, and liquids in infusion set can flow directionally at a certain rate, and all components are suitable for use in animal environment. The drop sensor and wireless module are optional. Optional functions of the software comprise Rate Mode and Anti-bolus function.

Since some parts and functions are optional, the veterinary infusion pump you purchased may not contain these additional parts and their relevant functions.

## 2.2 Host

### 2.2.1 Front View

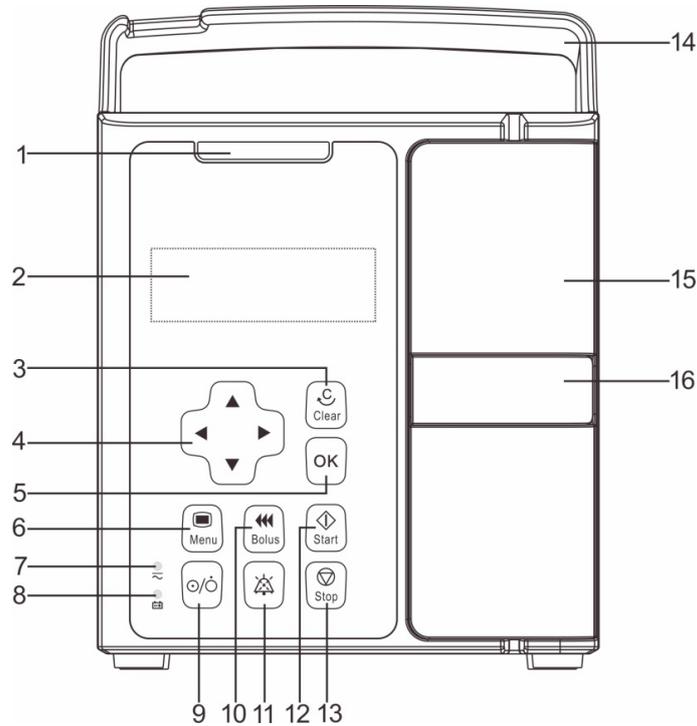


1.	<p>Alarm light</p> <p>The alarm light indicates different alarm levels in different colors and flash frequencies, please refer to <b>Chapter 7 Alarms</b> for details.</p>
2.	<p>Display</p> <p>Used for displaying infusion parameters and relevant content.</p>
3.	<p>&lt;CLEAR/BACK&gt;</p> <ul style="list-style-type: none"> <li>■ Under non-setting status, indicate to return to the previous menu or operation.</li> <li>■ Under the setting status, indicate to clear the current set or cancel the edit.</li> </ul>
4.	<p>&lt;DIRECTION&gt;</p> <p>Used for adjusting value, change lines and pages.</p>
5.	<p>&lt;OK&gt;</p> <p>Used for confirming input operation and saving values.</p>
6.	<p>&lt;MENU&gt;</p> <ul style="list-style-type: none"> <li>■ Under non-operation status, used for switching <b>[Main Menu]</b> interface and other interfaces.</li> <li>■ Under operation status, press and hold this key to lock; in locked state, press and hold to unlock.</li> </ul>

7.	<p>AC/DC indicator light</p> <ul style="list-style-type: none"> <li>■ On: The pump is connected to an AC/DC power supply (including shutdown).</li> <li>■ Off: The pump is not connected to an AC/DC power supply.</li> </ul>
8.	<p>Battery indicator</p> <ul style="list-style-type: none"> <li>■ Steady green indicates that the battery is charging.</li> <li>■ Flashing indicates that the battery is providing power.</li> <li>■ Light off indicates that there is no battery or the equipment is turned off and not connected to an AC power supply.</li> </ul>
9.	<p>&lt;POWER&gt;</p> <ul style="list-style-type: none"> <li>■ Used for turning power on, entering in standby state and turning off operations.</li> <li>■ When power off, press and hold (&gt;3 s) the key.</li> </ul>
10.	<p>&lt;BOLUS&gt;</p> <ul style="list-style-type: none"> <li>■ During infusion, press this key to enter the Bolus settings screen.</li> <li>■ When the pump is stopped, press this key to enter the Purge prompt screen.</li> </ul>
11.	<p>&lt;AUDIO PAUSED&gt; Pauses alarm sound.</p>
12.	<p>&lt;START&gt; After loading the infusion set correctly and completing setting infusion parameters, press this key to start the infusion.</p>
13.	<p>&lt;STOP&gt; During infusion, press this key to stop infusion. Infusion stops caused by alarms, such as occlusion and so on, press this key to cancel the alarm.</p>
14.	Handle
15.	Door
16.	<p>Door holder Pull it to open the door.</p>


---

## 2.2.2 Front View with the Door Opened

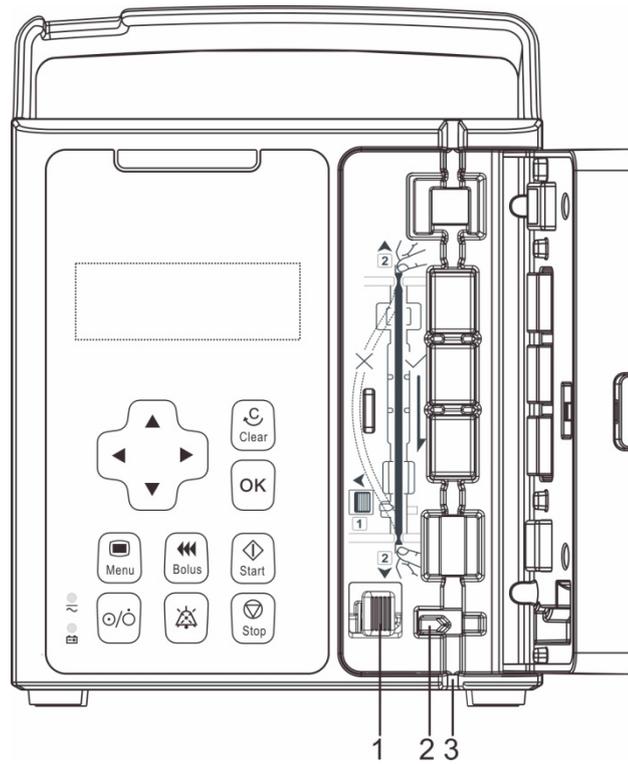

1.	Liquid check clip button
2.	Liquid check clip
3.	Infusion set slot


## 2.2.3 Rear View

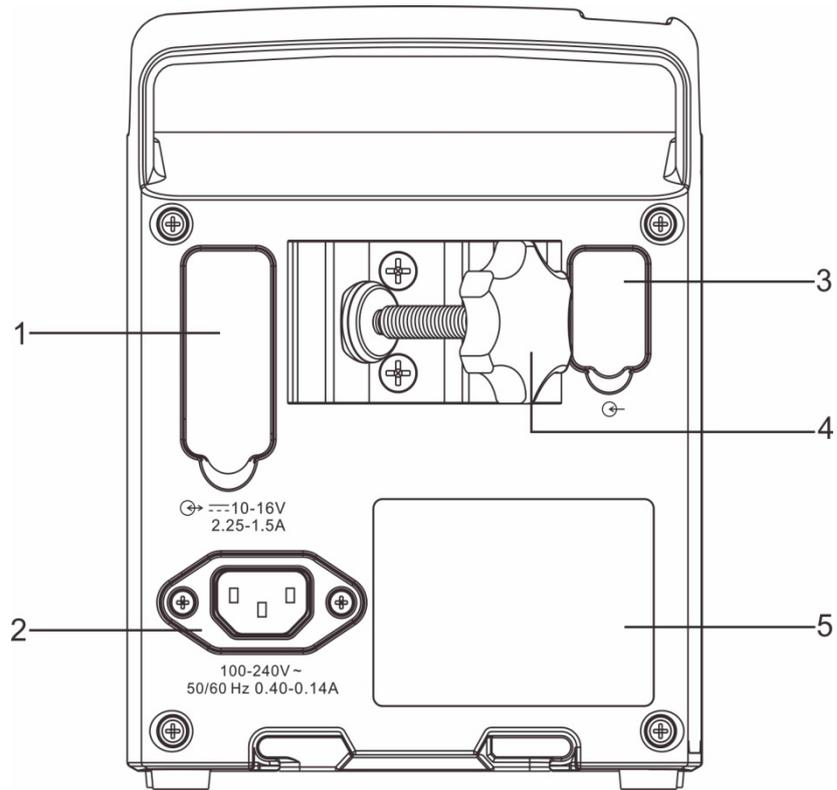

1.	<p>DB9 interface, which combines the following interface functions:</p> <ul style="list-style-type: none"> <li>■ DC power input interface</li> <li>■ RS232 interface</li> <li>■ Nurse call interface</li> </ul>
2.	<p>Alternating current power supply (AC) port Connected by three-core-type power cord and AC power source.</p>
3.	Drop sensor interface
4.	Pole clamp
5.	Product label

## 2.3 Screen Display

This veterinary infusion pump has a monochrome LCD screen. The display information comprises two main parts:

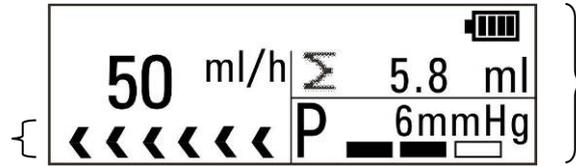

1.	<p>Parameter area</p> <p>Display battery icon, every parameter and the parameter value of the current screen, etc.</p>
2.	<p>Prompt bar</p> <p>Display run icon. The run icon on the screen displays the running operation:</p> <div style="display: flex; align-items: center; margin-left: 40px;"> <div style="margin-right: 20px;">     </div> <div> <p>The icon indicates normal running. Arrows move from right to left, and the running speed increases as the rate is increased.</p> <p>Motor stops caused by alarms during infusion, no icon.</p> </div> </div>

## 2.4 Cursor

In the main screen and parameter settings screen, when the cursor is located at an option or at a data value, the grounding of the option or the data value will turn to white

and the font will become blue. Press  or  to move cursor up or down and confirm the location. Press  to select the option or data value for further operation.

Note: Press  or  to "locate" cursor; press  to "Select".

# 3 Installation and Setting

---

---

## 3.1 Installation

---

### **WARNING**

---

- **Equipment assembly and refit (including correct protective grounding connection) during life period must be carried out by maintenance technicians whom are trained and licensed by the manufacturer, and evaluated according to the specified IEC60601-1. Please contact the company if you have any queries.**
  - **The software copyright for this equipment belongs to the manufacturer. Unless explicitly authorized, any alteration, reproduction or sale by any means or in any form by any organization or individual is prohibited.**
  - **All the analog equipment and digital facilities should be certified according to the specified IEC standard (such as: IEC60950 Information Technology Equipment Safety and IEC60601-1 Medical Electrical Equipment Safety). Moreover, all equipment should be connected based on the requirements of the valid version of the IEC60601-1 system. The qualified individual responsible for connecting auxiliary equipment to the input and output signal ports is also accountable for making the system in accordance with the IEC60601-1 standard. Please contact the company if you have any queries.**
  - **When this equipment combining with other electrical equipments forms a combination with a special function, and the user cannot determine whether there is an impending danger from each equipment specification (such as a danger of electric shock due to aggregation of current leakage), please contact the company or a specialist in the field at the pet hospital, to guarantee that all equipment in the combination are safe enough and will not be damaged.**
  - **Please make sure this equipment is securely fixed and positioned. Positioning changes and severe shock can lead to minor changes in the delivery accuracy.**
-

---

## NOTE

---

- This equipment is in accordance with the EN 1789:2007+A1:2010 standard. It can be fixed on cross bar (square cross bar: 10 x 25 mm) or vertical bar (round vertical bar with diameter size of 15-38mm) of ambulance with advanced pole clamp. Please refer to **3.1.3.2 Advanced Pole Clamp (Optional)** for detailed operation of advanced pole clamp.
- 

### 3.1.1 Out of Box Audit (OOBA)

Please check the packing case carefully before opening the box. If there is any damage, please contact the distributor or manufacturer immediately.

Please carefully remove the equipment and its accessories from the packaging in a correct manner, and inspect them against the packing list. Examine the equipment for any mechanical damage and ensure that the box includes all items on the packing list. Please contact the company if you have any queries.

## NOTE

---

- Keep the packing case and packaging materials for future transportation or storage.
- 

---

## WARNING

---

- They must be kept out of the reach of children. The packaging materials must be disposed of in compliance with local laws and regulations or the pet hospital policy on waste management.
  - The equipment may be contaminated by microbes during storage, transport and use. Please ensure that the package is undamaged before using, do not use if there is any damage.
- 

### 3.1.2 Operating Conditions

The operating environment of this veterinary infusion pump must meet the requirements in **A.1.2 Operating Environment**, and in accordance with the emergency medical care requirements of medical equipment short-time operation of the valid version of the IEC60601-1-12 system.

---

The operating environment should also be appropriately protected from noise, vibration, dust, and corrosive, inflammable or explosive substances. If installed inside the equipment case, a sufficient space before and after the equipment case should be ensured to facilitate operation, maintenance and repairing work. There should be a 2" (5 cm) gap around the veterinary infusion pump to ensure that air can circulate freely for a better cooling effect.

When the pump is transferred from one place to another, differences in temperature and humidity can cause condensation to form inside the pump. If this occurs, do not switch the pump to the "ON" state until the condensation has gone.

---


 **WARNING**

---


- **Please use only when the operating environment meets the requirements specified above. Otherwise, the pump's performance will not match the technical specifications in *A Product Specifications*. Device failure and other unexpected consequences may also result.**
- 

### 3.1.3 Mount the Clamp

#### 3.1.3.1 Standard Pole Clamp

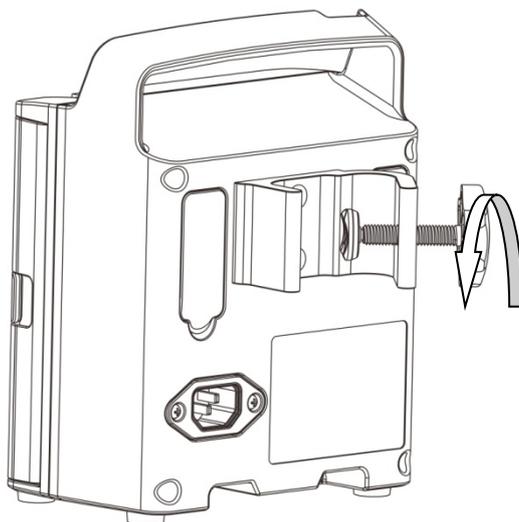


1. Turn counterclockwise to loosen the pole clamp until an IV stand can be inserted in.

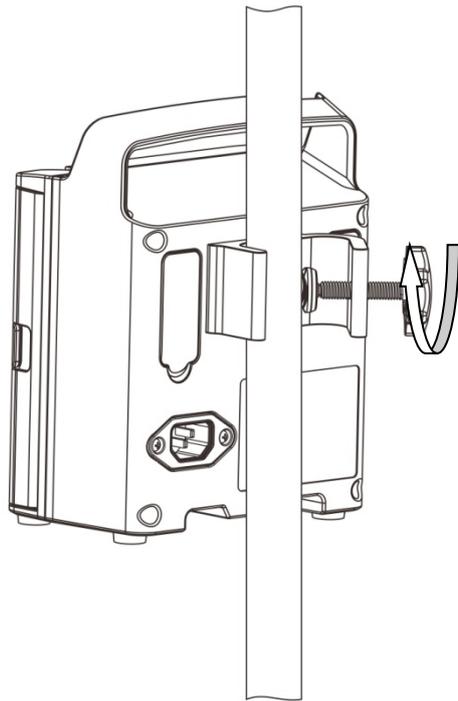

2. Tighten the pole clamp clockwise to firmly fix the device on the IV stand (round vertical bar with diameter size of 15-32mm).

### 3.1.3.2 Advanced Pole Clamp (Optional)

Press the button of pole clamp, horizontally or vertically adjust pole clamp, the button will pop-up after loosening the pole clamp. Turn the handle, pump can be fixed to cross bar (square cross bar: 10 x 25 mm) or vertical bar (round vertical bar with diameter size of 15-38mm).

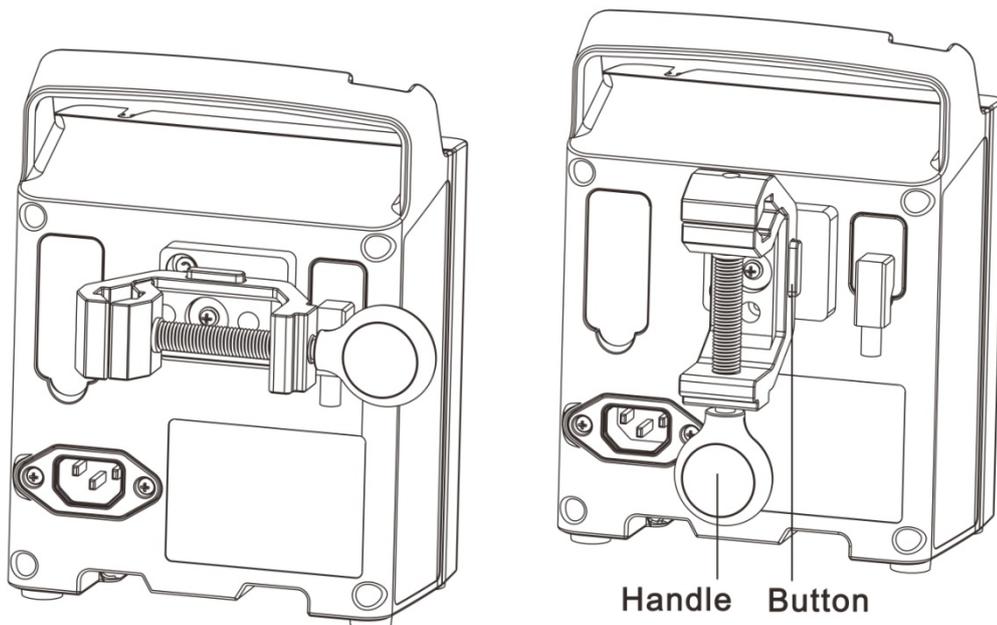

---

### 3.1.4 Connect the AC Power Source

1. Please confirm to use the original three-core-type power cord.
2. Insert one end of the power line into the AC socket on the back panel of the veterinary infusion pump.
3. Insert the other end of the power line into the matched three-plug connector connecting to the AC power.

---

#### **WARNING**

- **The earthing wire in the three-plug connector should be grounded. The connection of the protective earthing terminal of all fixed or permanently installed medical devices and external protective earthing system should be connected and verified based on the requirements of the valid version of the IEC60601-1-12 system. If there is a doubt whether the AC power system is grounded or not, please adopt the built-in battery and contact an electrical technician at the pet hospital or the company.**
- **Do not touch the power plug with wet or moist hands! If there is a liquid drug or residue on or around the power socket or plug, the user should completely clean and dry the area before plugging into the power supply, or accidents or injuries may result!**

---

#### **NOTE**


- **Compatible power supply: 100–240 V ~ , 50/60 Hz.**
- **The AC power cable should be correctly inserted and secured into the socket.**
- **Removing power cord is to disconnect equipment from power supply. Please ensure suitable clearance around the device to facilitate connect and remove power cord.**

---

### 3.1.5 Install and Operate the Drop Sensor (Optional)

#### **NOTE**

- **This section should be used with the optional drop sensor. The user may skip the instructions in this section if a drop sensor is not included with the veterinary infusion pump.**

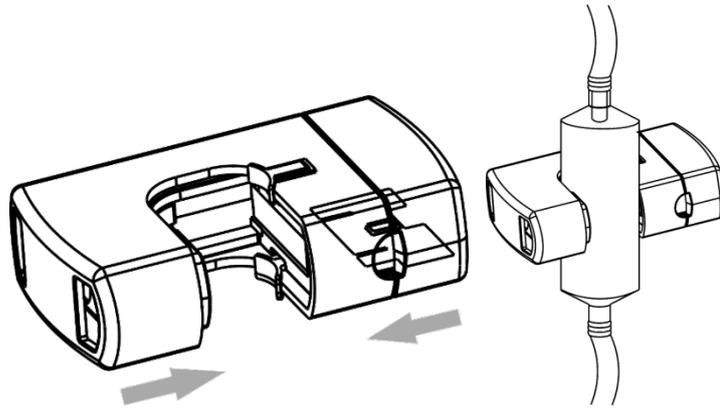

1. Firmly insert the signal line of drop sensor into the connecting port on the right side panel of the pump.
2. Clip the drop sensor to the drip chamber, making sure that the drop sensor is above the surface of the liquid.
3. Press  to start the infusion. The light of drop sensor flashes green when liquid is detected in normal infusion status.

---

## **WARNING**

- **For 60drop/ml infusion sets, it is recommended to set the rate <1000ml/h. Otherwise, the [Empty bottle] alarm will be triggered mistakenly.**
  - **Small liquid drops in drip chamber might be left on its wall after long time infusion, the medical staffs need to confirm and eliminate the drops. Otherwise, the accuracy of drop rate check will be affected, and the [Empty bottle] alarm will be triggered.**
-

---

## NOTE

---

- The surface of the liquid in the drip chamber must be lower than the drop sensor, which should be between 1/3 and 1/2 of the drip chamber.
  - The positioning block of the drip chamber must be inserted vertically through the positioning groove on the drop sensor.
  - Do not excessively tilt the drop sensor, or expose it to direct sunlight during infusion. Otherwise, accuracy of the drop sensor may be influenced.
  - Make sure that the drip chamber is not clamped too tightly by the drop sensor.
  - It is suggested that the single line of drop sensor should be changed every six months.
- 

## 3.2 Conventional Settings

This chapter only introduces the general settings for the veterinary infusion pump, please refer to other relative chapters for parameters and other feature settings.

### 3.2.1 Set Language

1. Select **[Main Menu]** **[Language]**.
2. Select **[Language]** from the **[Language]** according to actual needs.

### 3.2.2 Adjust Screen Contrast

1. Select **[Main Menu]** **[Brightness]**.
2. Select **[Brightness]**: 1-8. 8 for the brightest setting, and 1 for the darkest setting. When operating on battery power, you can set a low Contrast to save the power of the battery.

---

### 3.2.3 Set Date and Time

1. Select **[Main Menu] System Date and Time**.
2. Set **[Time]** and **[Date]**.

---

#### **CAUTION**

- **Please check the system date and time to keep accurate records in the History function.**
- 

### 3.2.4 Adjust Volume

1. Select **[Main Menu] Volume**.
2. Select **[Volume]:1-8.1** for the lowest volume;8 for the highest volume.

## 3.3 Restore Factory Default

During operation, you may change some settings in some situations. However, the changes may not be appropriate or correct, especially when animal or infusion set brands are changed. Therefore, you should restore the system to the default factory settings during operation according to actual needs, to guarantee that each configuration of the veterinary infusion pump is applicable for animal use. For some default factory settings of this equipment, please refer to **C Default Factory Settings**.


Select **[Main Menu] System Maintenance** Input User Maintenance Password **Restore factory default**, and restore the factory default settings as prompted on screen, some parameters will be restored to default values.

# 4 Basic Operation

---

---

## 4.1 Infusion Flow Chart

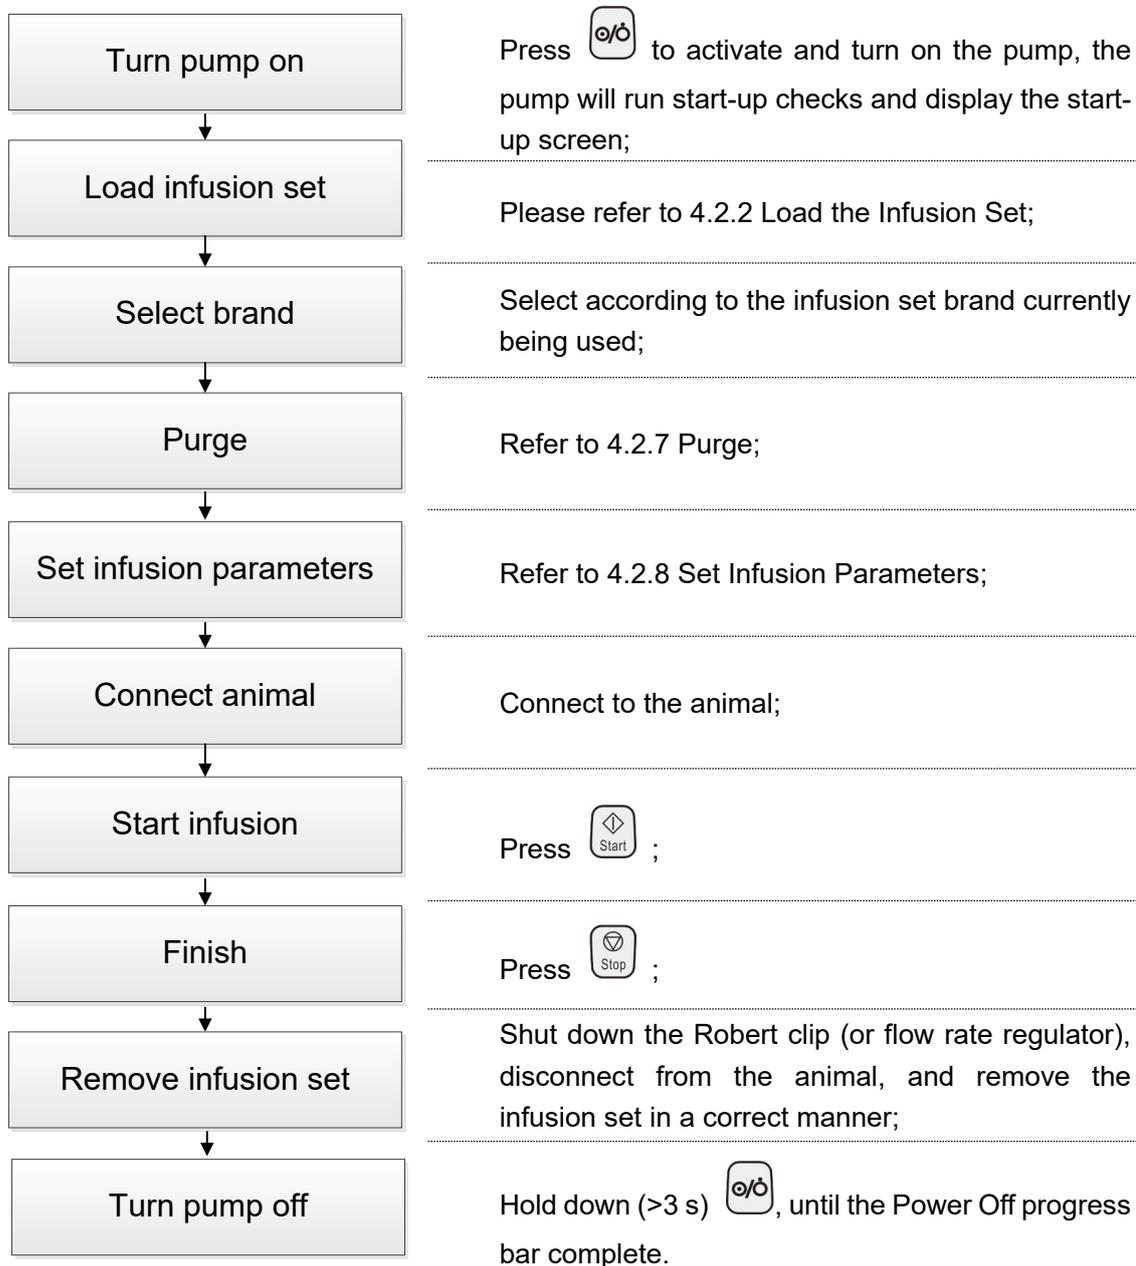

---

## 4.2 Operational Procedures

### 4.2.1 Turn on the Pump

Please turn on the device as the following steps:

1. Perform a safety inspection referring to **10.1 Inspection** before turning on the pump.
2. Press , the system will initiate the self-test and the screen will display the **[System Self-test]** interface:
3. The system will give out a sound "di" — indicating the self-testing of the loudspeaker to be successful.
4. The color of the alarm indicator lamp will change from red to yellow, turn on and off orderly — indicating the self-testing of the alarm lamp to be successful.
5. The system will give out a sound of "di" — indicating the self-testing of the buzzer to be successful.
6. Enter the operation interface after successfully completing the system self-test, and now you can operate the system through the key board.

---

#### **WARNING**

---

- **Please monitor the self-test process to make sure that the speaker, the alarm light, and the buzzer are all self-tested successfully. Otherwise, please contact the company and do not operate the pump until maintenance is performed.**
  - **Please contact the company if the veterinary infusion pump is damaged or cannot operate properly, and it cannot be used for animal infusion.**
- 

### 4.2.2 Load the Infusion Set


System will inspect whether infusion set is loaded after completing the self-test: If infusion set is loaded, enter the **[Infusion set selection]** interface; If infusion set is not loaded, enter the infusion set **[Installation Guide]** interface. If the infusion set is not

required to load, please press  to skip the step.


Load infusion set according to the following method:




1. Pull the door holder and open the door.

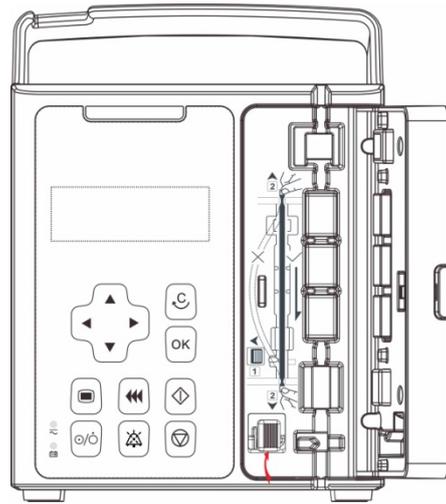

2. Pull the free flow clamp button upward left, and open the free flow clamp.

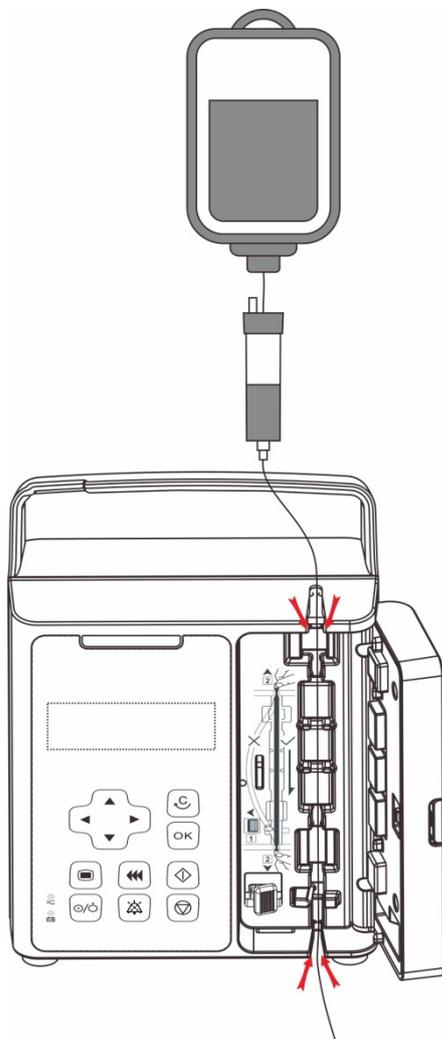

3. Load the set, confirm it is firmly loaded into the tube slot.

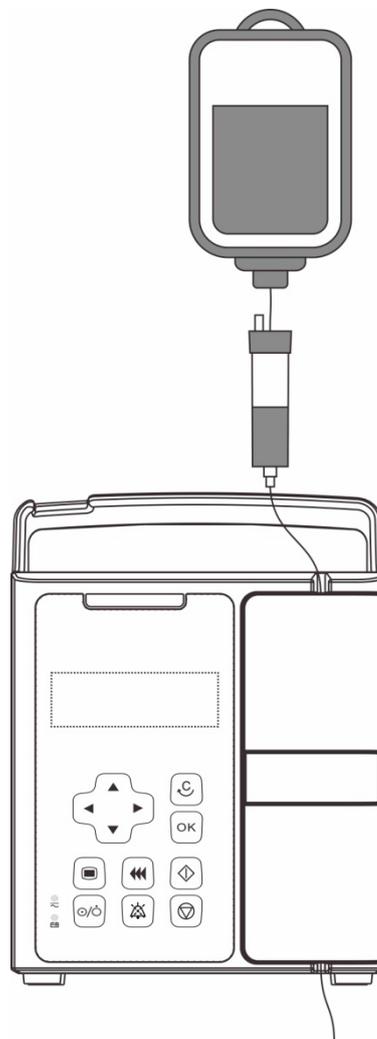

4. Close the door, the interface will enter **[Infusion set selection]** interface, indicating that the infusion set is loaded correctly; otherwise, it needs to be

---

reloaded.

---

## **WARNING**

---

- The infusion set should be firmly loaded into the slot, and not jutting on the outside of the slot.
  - Before using this veterinary infusion pump, the veterinary infusion pump, infusion set, and other accessories should be loaded correctly.
- 

### 4.2.3 Change the Infusion Set

Follow the steps below to change the infusion set:

1. To prevent animal injury due to free flow, before changing the infusion set or extruded tube, please shut down the Robert clip (or flow rate regulator). During infusion, press  to stop the pump.
2. Pull the door holder, open the door, pull the free flow clamp button upward left, and take out the loaded infusion set.
3. Please refer to **4.2.2 Load the Infusion Set** to reload the infusion set.

### 4.2.4 Change the Infusion Bottle (Bag)

Follow the steps below to change the infusion bottle (bag):

1. To prevent animal injury due to free flow, before changing the infusion bottle (bag), please shut down the Robert clip (or flow rate regulator). During infusion, press  to stop the pump.
2. Take out the loaded infusion bottle (bag), and reload it.

### 4.2.5 Select Infusion Set Brand

On the [Infusion set selection] screen, press   to select the infusion set brand, and press  for confirmation. Specific brand, please refer to **5.8 Common Infusion Set Brands**.

---

## **CAUTION**


---

- Please confirm that the current selected brand is the same as the brand actually used.

## 4.2.6 Infusion Mode

### ■ Unit of Rate (ml/h)


Press  to exit [Main Menu], and enter the [Rate Mode Setting/Running] interface.

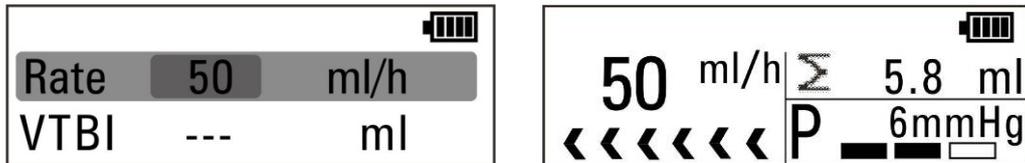

Mode	Parameters	Parameter Range
Rate Mode	Rate	0.1 - 1500ml/h
	VTBI	0.1 - 9999ml

### ■ Unit of Rate (drip/min)

1. Select [Main Menu] [Drip setting].
2. Select [**drip/min** On], and set the “drip”. If [Off] is selected, the following steps cannot be conducted.
3. Press  to exit [Drip setting] interface, and enter the [Rate Mode Setting] interface.
4. Change the unit of Rate to “drip/min”, set the parameters, and then press  to start the infusion.

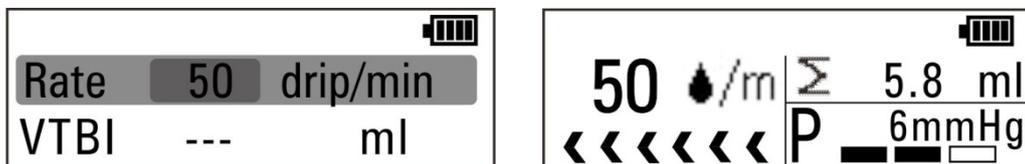

Mode	Parameters	Parameter Range
Rate Mode	Rate	1 - (400*drip/60) drip/ min
	VTBI	0.1 - 9999ml

---

## 4.2.7 Purge

During infusion, the user should prevent air bubbles from entering the blood with the liquid drug, which may form an aeroembolism and put animals in serious danger. Therefore, air bubbles in the infusion set should be eliminated before the infusion.

On infusion parameters setting interface, press  to enter [Purge] prompt screen. Hold down  to enter [Purge] running screen, release  after the air bubbles are purged.

---

### WARNING

- **During the purge, please disconnect the pump from the animal.**  
**Otherwise, the animal will be in serious danger!**

---

### NOTE

- Purge rate can not be changed.
- [Air in line] alarm will not be triggered during purge.

---

## 4.2.8 Set Infusion Parameters

Under rate mode, users can set infusion parameters by pressing , , , , and .

---

## 4.2.9 Infusion

When ready, connect the infusion set to the animal. Press  to start the infusion, and the screen will display the running icon, the arrows will move from right to left, and the running speed will increase, which will indicate that the rate will also increase.

---

### WARNING

- **Users should regularly monitor the connection between the infusion set, pump and animal, and infuse according to the method mentioned in the manual.**

---

## NOTE

---

- When in running status, if there is no operation in other interface over 2 minutes, it will return to the running screen automatically.
- 

### 4.2.10 BOLUS

In run screen of rate mode, press  to enter [Bolus] settings screen. Follow the ways to start the bolus:

- **Manual Bolus:** Set [Bolus] rate, and then press and hold  to start a manual bolus. The system returns to the original rate when  is released, or  is hold for 10 seconds.

## NOTE

---

- If the previous bolus rate  $\leq$  current rate, the default bolus rate is 600ml/h.
  - If no operation is performed within 2 minutes, the veterinary infusion pump will automatically exit the Bolus Settings screen and the procedure must be repeated.
  - [VTBI Near Done] alarm will not be triggered during bolus.
  - Occlusion pressure will automatically switch to "High" level when bolus, animal's clinical condition and working condition of the veterinary infusion pump must be monitored carefully.
- 

### 4.2.11 Change the Rate during Operation

In run screen of rate mode, press ,  or  to change the value of the [Rate] into the adjustable state, thus to set the expected rate, press  or  again for confirmation, then start to infuse under the new set rate.

---

## 4.2.12 Complete

When [VTBI] is not set during the infusion and infusion is completed, if drop sensor is installed and the switch of [Drip rate check] is on, the [Empty bottle] alarm will be triggered; if drop sensor is not installed, the [Air in line] alarm will be triggered.

When [VTBI] is set during the infusion and the remaining infusion time is close to the [Near end] time set by the users, the [VTBI Near Done] alarm will be triggered. If no action has been taken, the alarm will not be canceled automatically until the infusion is completed, and then switch to [VTBI Done] alarm. Set [Near end] time, please refer to **5.7 Time Near End**. When infusion is completed, enter to [KVO] mode, and KVO mode will run for 30 mins at most. Infusion will stop automatically after the KVO is finished, and the [KVO Finish] alarm will be triggered. Set KVO rate, please refer to **5.1 KVO**.

## 4.2.13 Standby

Under non-operation status, tap (<3 s)  to enter [Standby] interface, default display the previous standby time, press  to modify standby time (range is 00:01-99:59 hh:mm), press  for confirmation after modifying. The pump cannot be put in standby mode if there is a high-level alarm.

When the standby state is ended, the title bar will display [Standby Time Expired], press  to confirm quit, and the screen will enter to the interface before standby appears. Press  to remain in standby status.

## 4.2.14 Turn off the Pump

Follow the steps below to turn off the veterinary infusion pump:

1. Disconnect from the animal;
2. Hold down (>3 s) , until the Power Off progress bar complete, and the power will turn off.

---

## **NOTE**

- **The current operating data and saved data will always be autosaved when the device is powered off properly. The effective storage duration of the data is equal to the service life of the device.**
-

---

FOR YOUR NOTES

# 5 Setting Parameters

---

---

## 5.1 KVO

KVO (Keep Vein Open) means to keep the vein open, during which the veterinary infusion pump continues infusion at a very low rate after finishing the infusion in order to prevent blood backflow or vascular occlusion.

Select **[Main Menu]** **[KVO rate]**: 0.5ml/h is unadjustable.

## 5.2 Occlusion Pressure

Occlusion pressure is adjustable, which can meet the requirements for occlusion pressure of different animals during infusion. Pressure in the infusion tube can be measured by the built-in pressure sensor, pressure can be calculated by the internal CPU, which is compared with the preset occlusion alarm threshold. **[Occlusion]** alarm will be triggered if pressure exceeds the threshold.

### 5.2.1 Set Occlusion Pressure

1. Select **[Main Menu]** **Occl. pressure]**.
2. Occlusion pressure Degree 3, lowest at 150mmHg, and highest at 900mmHg. Occlusion pressure should be selected according to actual needs.

---

### CAUTION

---

- **If the animal experiences discomfort at a higher occlusion pressure, monitor the animal's physical conditions under the higher occlusion pressure closely, and take measures instantly if any abnormal condition occurs.**
  - **When the infusion set with ultrafilter at a lower occlusion pressure, the [Occlusion] alarm might be triggered at high rate due to resistance generated from liquid flow of ultrafilter. Select a higher occlusion pressure or lower rate to cancel alarm.**
-

---

## 5.2.2 Set Pressure Unit

1. Select [**Main Menu**] **Pressure unit**].
2. Select [**Pressure unit**]: The 4 various forms of pressure units, mmHg, kPa, bar and psi are converted automatically, and can be selected according to actual needs.

---

### CAUTION

---

- Carefully confirm the edit when changing the current pressure unit.
- 

## 5.2.3 Dynamic Pressure Scanning (DPS)

During the infusion, the bottom-right corner of the Run screen demonstrates real-time pressure changes of the animal, in order to find the cannula occlusion at an earlier time and to prevent the occurrence of further complications.

The pressure icon **P**  on the screen indicates the condition of the current pressure:

- 1 solid area indicates low occlusion pressure
- 2 solid areas indicate medium occlusion pressure
- 3 solid areas indicate high occlusion pressure

## 5.2.4 Automatic Pressure Release Function (Anti-Bolus)

When occlusion occurs, infusion will stop and the [**Occlusion**] alarm will be triggered. After the alarm is triggered, the motor is reversed, and the cannula pressure is then released. This prevents an additional aggressive dose to the animal after the occlusion is eliminated.

## 5.3 Set the Air Bubble Size

Air bubble size indicates the size of air bubble that can be monitored in the tube. The lower of the bubble size, the smaller air bubble can be identified. Bubble in the infusion tube can be measured by the built-in ultrasonic sensor, bubble size can be calculated by the internal CPU, which is compared with the preset threshold. [**Air in line**] alarm will be triggered if bubble size exceeds the threshold.

1. Select [**Main Menu**] **[Bubble size]**].

- 
2. Select [**Bubble size**], five levels of air bubble can be selected, lowest at 50 l, and highest at 100 l. Air bubble level should be selected according to actual needs.

---

## CAUTION

- If the animal experiences discomfort or danger at a higher air bubble filter level, monitor the animal's physical conditions and select the actual needed level. Measures should be taken instantly if any abnormal condition occurs.
- 

## 5.4 Acumulated Bubble

1. Select [**Main Menu**] [**Accum. bubble**].
2. Select [**Accum. bubble**]: 0.1-4.0ml/h is adjustable.

## 5.5 Key Lock Function

When locked, an  icon in the upper-right corner of the screen merges. The following are two ways for automatic locking and manual locking:

- Automatic Locking:
  1. Select [**Main Menu**] [**Auto-lock**].
  2. Select [**Auto-lock**]: Off, 1-5min. After a specific time is set during the running state, and if there is no operation or high-level alarm within the set auto-lock time, the key board will be auto-locked. [**Off**] indicates closing automatic locking function.
- Manual Locking: In the running interface, under the unlocking condition, press and hold  (>3 seconds) to lock the key board.

If unlocking is needed, press and hold  (>3 seconds) to unlock, it is automatically locked during the high-level alarm.

## 5.6 Reminder Function

1. Select [**Main Menu**] [**Reminder**].
2. Select [**Reminder**]: Off, 1-5min. After a specific time is set, the infusion set is loaded. If no operations are performed to the pump within the set time (including operations on the keyboard, the slider and the pull handle), and the [**Reminder**]

---

alarm will then alert the user to proceed to the next step. **[Off]** indicates closing the function.

## 5.7 Time Near End

1. Select **[Main Menu] Near end**].
2. Select **[Near end]**: Off, 1-30min (when <10min, the stair-step is 1min, and when 10min, the stair-step is 5min). After a specific time set, when the remaining infusion time is close to the **[Near end]** set by the users, **[VTBI Near Done]** alarm will be triggered. **[Off]** indicates closing the function.

## 5.8 Common Infusion Set Brands

There are multiple commonly used infusion set brands installed inside the veterinary infusion pump, making it convenient for the user to select from. For specific infusion set brands, please refer to actual infusion device.

1. Select **[Main Menu] Commonly used tube**].
2. Select in **[Commonly used tube]** according to actual needs.

Note: Please ensure that at least one “Commonly used tube” to be selected.

Recommended Infusion Sets List

No.	Infusion Set Brand	Specifications and Model
1	B. Braun	Intrafix SafeSet
2	SK	ZPQ, JMB,150ml, SK-B

---

### **WARNING**

---

- **This equipment has to be used with high elastic tube. If you are not sure whether the tube is high elastic tube, please contact us for tube test.**
- 

## 5.9 Bed No. Settings

1. Select **[Main Menu] [System Maintenance] Input User Maintenance Password Bed No.**].
2. Select **[Bed No.]**: 1-999. [---] indicates invalid values. Beds can be differentiated through setting Bed No.

---

## 5.10 View Department

The veterinary infusion pump are net-connected with BeneFusion CS5 Infusion Supervision System through the approach of wireless networking, and the system contains department information, the system will automatically distribute department information to all veterinary infusion pumps when pumps are on.

Select **[Main Menu] System Maintenance** Input User Maintenance Password **Department]** to view the department information.

## 5.11 Set the Sensitivity of Empty Bottle Alarm

1. Select **[Main Menu] Empty Alarm**.
2. Select **[Empty Alarm]: High** and **Low**. **[High]** indicates high sensitivity of **[Empty bottle]** alarm detection, **[Empty bottle]** alarm will be triggered in shorter time; **[Low]** indicates low sensitivity of **[Empty bottle]** alarm detection, **[Empty bottle]** alarm will be triggered in longer time. It can be selected according to actual needs.

Note: **[Empty Alarm]** option is not visible when the switch of **[Drop sensor]** is off.

---

FOR YOUR NOTES

# 6 Other Functions

---

---

## 6.1 Nurse Call

Select **[Main Menu] System Maintenance]** Input User Maintenance Password **Nurse call]**, and set in the open menu:

- Switch

On: indicates the opening of the nurse call function.

Off: indicates the closing of the nurse call function.

- Signal type

1. Cont.

Indicates that the output nurse call signal type is the same as that of the alarm existence time, i.e., from the occurrence of the alarm to the end of it.

2. Pulse

Indicates the output nurse call signal is a pulse signal with the type of 1 second. When several alarms exist at the same time, only one pulse signal can be outputted. If the current alarm is not removed and another alarm occurs, then one additional pulse signal is outputted.

- Trigger type

1. Normally Closed: Select when the pet hospital call system is set as **[NC]**.

2. Normally Open: Select when the pet hospital call system is set as **[NO]**.

- **Alarm level: Three options: [High], [Medium] and [Low].The system sends nurse call signals according to the alarm at the selected alarm level or above.**

---

### **WARNING**

---

- **Non-veterinarians are forbidden to modify the nurse call setting.**
  - **The nurse call function must be used in conjunction with a special cable.**
-

---

## NOTE

---

- **Veterinarians should not consider the nurse call function as the main alarm notice approach, and rather combine the sound and visual alarms of the veterinary infusion pump and the performances and symptoms of the animal in order to judge the animal's conditions and take further attention as needed.**
- 

## 6.2 Wireless Networking (Optional)

The veterinary infusion pump can be configured with the wireless modules, and be net-connected with BeneFusion CS5 Infusion Supervision System through the approach of wireless networking. Through the network:

- The veterinary infusion pump sends real-time infusion parameters, alarm information, prompt information, Bed No. and other information to BeneFusion CS5 Infusion Supervision System.
- BeneFusion CS5 Infusion Supervision System and veterinary infusion pump can display synchronously. For detailed descriptions, please refer to the instructions of BeneFusion CS5 Infusion Supervision System (hereinafter called CIMS).

Normal communication of the pump and CIMS depends on whether the network connection is successful, operators are unable to observe the operation status of the pump in real time when the communication is interrupted. After the network connection settings of the pump and CIMS are modified, operators shall reset the network connection as required in the manual to ensure the communication of the pump and CIMS are restored.

When using wireless modules to connect to the Internet while using the veterinary infusion pump, the wireless icon on the upper-right corner indicates the working condition of the wireless modules:



Wireless modules work in order

No  
icons

No wireless modules configured or connect BeneFusion  
CS5 Infusion Supervision System

---

## NOTE

---

- **Wireless security transmission distance is no more than 50 meters.**
  - **2.4 GHz Wi-Fi frequency range, WEP and WPA/WPA2 security modes and 802.11b/g/n wireless standard are supported.**
  - **The settings of the wireless network must be conducted by technicians approved by the company or maintenance staff designated by the company.**
- 

## 6.3 Data Export

To export the data in the veterinary infusion pump, please refer to the following steps:

1. Log on PC tools, and connect the PC to the veterinary infusion pump;
2. When the veterinary infusion pump is in working communication with the PC, the PC automatically reads all the data in the pump;
3. Select [**History Record**] in PC tools;
4. Export data.

## 6.4 WLAN Setting

The pump can be net-connected through built-in Wi-Fi module.

1. Select [**Main Menu**] **WLAN Setting**], then select [**On**] to enable Wi-Fi function.
2. Select [**Advanced Settings**], there are two ways to distribute IP address:
  - DHCP: Check the checkbox to activate DHCP, IP address, subnet mask and gateway can not be modified, automatically obtain an IP address.
  - Manually: Uncheck the DHCP checkbox, enter IP address, subnet mask and gateway.
3. Available networks shall be displayed:
  - If password is required for to-be-connected network, please enter the password.
  - If password is not required for to-be-connected network, you can connect the network directly.

---

FOR YOUR NOTES

# 7 Alarms

---

---

The alarm is used in order to alert the veterinarian by means of sound and light when abnormal situations occur during the infusion procedure which can lead to infusion changes or when the infusion of the animal cannot continue due to the unexpected breakdown or pause/delay of the veterinary infusion pump.

---

## WARNING

---

- It is potentially hazardous to use the same or similar equipment with different alarm presets within the same area.
- 

### 7.1 Alarm Level

According to the severity scale of the alarm, the alarms of the veterinary infusion pump can be classified to high-level alarms, mid-level alarms and low-level alarms.

### 7.2 Alarm Types

When an alarm is triggered, the veterinary infusion pump will use the following visual and audible methods to alert the user:

- Visible alarms
- Audible alarm
- Alarm Information

Among the visible alarms and audible alarms, the alarm information will distinguish alarm levels in different ways.

Alarm level	Color of alarm light	Audible alarm frequency	Flashing light frequency	Light/no-light ratio
High-level alarms	Red	10 seconds	2.0±0.6Hz	20%-60%
Mid-level alarms	Yellow	15 seconds	0.6±0.2Hz	20%-60%

Low-level alarms	Yellow	20 seconds	Steady	100%
------------------	--------	------------	--------	------

## 7.2.1 Multi-level Alarm Rules

When several alarms occur simultaneously, the alarms proceed according to the following rules:

- When several alarms at different levels occur, the visible alarms and audible alarms are consistent with the highest-level alarms.
- When several alarms at different levels occur, only the highest-level alarm is displayed, and after it is cancelled, the lower-level alarm will then be displayed.
- When several alarms at the same level occur, the alarm information will be demonstrated in an alternate manner.

The title bar of the veterinary infusion pump screen will display the corresponding alarm information during the alarm blast, to see more details in ***D Alarm Information***.

### NOTE

- **The [No Communication] alarm of the pump and BeneFusion CS5 Infusion Supervision System are delayed for 3 minutes, while other alarms are delayed for less than 5 seconds.**

## 7.3 Alarm Handling Rules

Under normal working conditions, when an alarm occurs, all the alarm types of the veterinary infusion pump will alert according to their respective alarm levels. In addition, the user can pause the alarm sound according to demands.

- For high level (except battery empty) and medium level alarms, press  to pause alarm sound for 2 minutes, no alarm sound is made in any case. When the alarm pause time expires, the alarm tone will sound. Press  to cancel high level alarms (except battery empty and system error).
- For low level alarms, press , no alarm sound, alarm information and alarm light, until it is triggered next time.

### NOTE

- **[Battery Empty] alarm sound is unable to be paused.**

---

## 7.4 Alarm Countermeasures

---

### **WARNING**

---

- **When an alarm is triggered, the animal's condition should be checked firstly and operation should only be allowed to proceed after the reason for the triggering of the alarm is ruled out.**
- 

When an alarm is triggered, please follow these steps and take appropriate action:

1. Check the animal;
2. Check the alarm type and the parameter which triggered the alarm;
3. Determine the reason for the alarm;
4. Eliminate the reason for the alarm;
5. Check whether the alarm has cleared.

### **NOTE**

---

- **Please refer to *D Alarm Information* for specific handling procedures for each alarm.**
  - **The operator position shall be the normal operating position of the veterinary infusion pump (0.5m). Otherwise, operators might identify alarm mistakenly.**
-

---

FOR YOUR NOTES

# 8 Battery

---

---

## **WARNING**

---

- **The battery can not be disassembled. The battery should be changed by maintenance staff designated by the company only. Inserting fuel cell or changing battery by personnel who has not received suitable training may cause such danger as overtemperature, fire or explode.**
- 

The veterinary infusion pump is configured with rechargeable Lithium batteries to ensure that the veterinary infusion pump can be used normally under the condition of the animal's migration within the pet hospital or during the circumstance of a power failure. When the veterinary infusion pump switches to the AC power, the battery can be charged regardless of whether the veterinary infusion pump is on or off. The battery is chargeable only within the veterinary infusion pump. During charge, the battery icon in the upper-right corner of the screen floats left and right. If the battery icon stops floating and is completely filled, it indicates that the battery is fully charged. Under the condition of a sudden power failure, the pump will automatically use the battery to provide power as a backup.

The battery icon on the screen indicates the condition of the battery:



The battery jar of the veterinary infusion pump is installed with batteries, and the white fill area indicates the quantity of electricity.



Low battery electric quantity indicates that charging is needed.



When the battery is empty, charging is needed immediately.

The power supply by the battery can only be sustained for a limited period of time. The **[Battery Empty]** alarm will be triggered when the battery voltage is too low, and red alarm light will flash. The alarm will continue within the remaining time of the battery's electric quantity and cannot be paused. Now, the veterinary infusion pump should be switched on to AC power for charging.

---

## 8.1 Battery Performance Optimization

When the battery is used for the first time, at least two complete optimizing cycles should be ensured. A complete optimizing cycle contains the following: Charging incessantly, and then discharging until the power of the veterinary infusion pump runs out. During usage, regularly optimizing the battery performance will extend its lifespan. It is suggested that the battery should be optimized when in use or in storage for three months, or when the running time of the battery is significantly shortened.

Please follow the steps below during optimization:

1. Disconnect the pump from the animal and stop the infusion.
2. Switch the veterinary infusion pump on the AC power and charge the battery incessantly for over 10 hours.
3. Disconnect the AC power and use the battery to charge the veterinary infusion pump until the veterinary infusion pump is closed.
4. Switch the veterinary infusion pump over to AC power again and charge the battery incessantly for over 10 hours.
5. The battery optimization is now complete.

## 8.2 Check the Battery

The performance of the battery may decrease over time. Please follow the steps below when checking the battery:

1. Disconnect the pump from the animal and stop the infusion.
2. Switch the veterinary infusion pump on the AC power and charge the battery incessantly for over 10 hours.
3. Disconnect the AC power and use the battery to charge the veterinary infusion pump until the veterinary infusion pump is closed.
4. The length of the battery's lifetime reflects the performance of the battery.

Note: If the length of the battery's lifetime is obviously shorter than that claimed in the specifications, please consider changing the battery or contact us.

---

## NOTE

---

- The lifespan of the battery depends on how frequently it is used and on how long it has been used, battery capacity decreases with increase in charging and discharging times. If the maintenance and storage of the battery is appropriate, the lifespan of the Lithium battery is no less than 300 times of full charging and discharging. If the use of battery is improper, its lifespan shall be shortened or in failure status. We recommend replacing the lithium battery every 3 years.
  - Please connect to the AC power source if [Battery Empty] alarm is triggered. To prevent battery not used for a long time or in battery empty status, if battery is not charging more than two months after battery is empty, battery will be in failure status. Do not charge the failure battery, and replace the failure battery.
  - If battery will not be used for a long time, we recommend keeping the battery in a fully charged state and charging the battery every two months for lifespan guarantee. Please replace the battery if the length of its lifetime is obviously shortened during optimization.
  - The length of the battery's lifetime depends on the device configuration and operation, for example: Under the condition of the power supply by the battery, frequent infusion at a high rate will also shorten the length of the battery's lifetime.
- 

## 8.3 Battery Recycling

If there is any obvious damage to the battery or to the battery capacity exhausts, it should be replaced and recycled appropriately. Please follow the applicable laws on recycling.

---

### **WARNING**

---

- The battery must not be disassembled, burned or short-circuited. Burning, exploding or leaking batteries can cause animal injury.
-

---

FOR YOUR NOTES

# 9 Preservation and Sanitation

---

---

The pump must be cleaned or disinfected using the materials and methods listed in this section. The manufacturer will not be responsible for any damage or accident caused by cleaning and disinfection using other materials and methods.

The manufacturer shall not be held responsible for the efficacy of the following chemicals or methods for infection control. Please contact your pet hospital's infection prevention department or epidemiology specialists for advice on infection control practices.

## 9.1 Description

Please make sure that your device and other fittings are clean without dust. In order to prevent any damage to the device, please abide by the following rules:

- Dilute all cleaning agents and disinfectants in accordance with the manufacturer's instructions, or use as low a concentration as possible.
- Do not immerse or submerge the device in liquid.
- Do not pour liquid on the device or accessories.
- Avoid liquid from entering the pump body.
- Do not use abrasive materials (such as steel wool or silver polishes), or any strong solvent (such as acetone or any detergent containing acetone).

---

### **WARNING**

---

- **Turn off the pump and disconnect the AC power source line from the socket before cleaning. Do not clean and disinfect the device, export history record and perform other operations when animals are using the pump.**
- 
- 

## 9.2 Cleaning

The pump should be cleaned regularly. If operating in dirty or sandy areas, cleaning should be more frequent. Before cleaning, please consult or refer to the pet hospital's specific regulations concerning medical device cleaning.

The recommended detergents include: Hydrogen peroxide (3%).

---

To clean your equipment, follow these rules:

1. Turn off the pump and disconnect the AC power source line.
2. Wipe the display screen after soft cotton balls absorb an appropriate amount of detergent.
3. Use a piece of soft cloth which absorbs a modest amount of cleaning agent to wipe the surface of the device.
4. When necessary, use a piece of cloth to wipe off any excess cleaning agents.
5. Place the pump in a cool and ventilated environment to dry.

## 9.3 Disinfection

The operation of disinfection may cause certain damage to the veterinary infusion pump. You are recommended to disinfect only when it is necessary in your desired maintenance plan. Clean the equipment before disinfection.

The recommended disinfectants include: glutaraldehyde-type 2% liquid disinfectant.

---

### CAUTION

- **Never use EtO or formaldehyde for disinfection.**
  - **Do not conduct high pressure or high temperature disinfection for the veterinary infusion pump and its accessories.**
-

# 10 Maintenance

---

---

## WARNING

---

- **The pet hospital or medical facility using this veterinary infusion pump must set up a comprehensive maintenance plan. Failure to do so may result in equipment failure or other unexpected consequences, and may even jeopardize animal safety.**
  - **All safety inspections or maintenance work involving the disassembly of the device must be conducted by professional maintenance personnel. Actions by unqualified persons may result in device failure and may even jeopardize animal safety.**
  - **Please contact the company immediately if you encounter problems with the device.**
- 

## 10.1 Inspection

The veterinary infusion pump must be given a thorough inspection before use, after 6-12 months of continuous use, and after maintenance or upgrades, to ensure that it is operating and functioning normally.

The inspection criteria are:

- The environment and power supply meet requirements.
- The equipment and accessories have no mechanical damage.
- The power cord is not damaged and has sufficient electrical insulation.
- Accessories used with the pump are correct.
- The alarm system functions correctly.
- Battery performance.
- Self-checking and pump functions are normal.

If there are any forms of damage or abnormal circumstances, do not use the veterinary infusion pump and contact the company immediately.

---

## 10.2 Maintenance Plan

The following tasks must be conducted by professional maintenance personnel approved by the company. Please contact the company if the following maintenances are needed. Must clean and disinfect the device before the test or maintenance.

Inspection/Maintenance Items	Frequency
Perform a safety inspection according to the IEC60601-1 standard.	Once every two years. Perform after the board is changed or the veterinary infusion pump is accidentally dropped.
Preventive maintenance (refers to the Maintenance Manual for pressure calibration, sensor calibration, and pump inspection).	Once every two years, or when you suspect the occlusion alarm is abnormal, the flow volume is inaccurate, or the infusion set is incorrectly identified.

## 10.3 View Information

Select **[Main Menu]** **[Version Information]**. In the **[Version Information]** interface, you can view the information of the version of the veterinary infusion pump system software and other versions.

## 10.4 Safe Disposal and Recycling

Please contact the company for related information about safe disposal and recycling.

# 11 Accessories

---

---

## **WARNING**

---

- **Use the accessories specified in this chapter only. Other accessories may cause damage to this veterinary infusion pump, or cannot reach the specification in this manual.**
  - **Please do not replace an accessory if its package or itself is damaged.**
- 

Materials	PN
Power cord (Select PN according to sales area)	0020-20-12522
	009-002755-00
	009-002756-00
	009-002757-00
	009-002758-00
	009-003358-00
	009-003651-00
009-002758-00	
Standard pole clamp	115-031551-00
Advanced pole clamp	115-031552-00
Nurse call cable	115-034140-00
RS-232 communication cable	115-034142-00
DC input cable	115-034144-00
Drop Sensor	115-013821-01
Floor model infusion stand	034-000321-00
Multi-channel pump stand	045-001434-00
Pet bracket	115-033273-00

---

## **NOTE**

- **This Operator's Manual describes the most complete functional configuration of the system. The device you are using may not have some of the settings or functions described herein.**
-

# A Product Specifications

---

---

## A.1 Safety Specifications

### A.1.1 Product Classification

Classifications of this veterinary infusion pump according to the IEC60601-1 standard are as follows:

Safety	
Components	Host
Type of protection against electrical shock	I
Degree of protection against electrical shock	CF Protected against defibrillation
Ingress Protection	IP34
Explosion protection level	Unsuitable
Mode of operation	Continuous
Mobile level	Portable

NOTE:

- I: Type I devices
- CF: Class CF applied parts, can be directly used in the heart.
- IP34: Protected against solid foreign objects with a diameter no less than 2.5mm and protected against spraying water.
- Unsuitable: The equipment is not suitable for use in the presence of a flammable anesthetic mixture with air or with oxygen or nitrous oxide.
- Portable devices: Can be moved from one place to another by one or more persons or by other means when the devices are in use or being used.
- Portable veterinary infusion pump: Used to control the infusion of animals and are devices which can be carried by the animals continuously.

## A.1.2 Operating Environment

<b>Work environment</b>	
Temperature	5 - 40°C
Relative Humidity	15 - 95%, non-condensing
Atmospheric pressure	57 - 106 kPa
<b>Storage environment</b>	
Temperature	-20 - 60 °C
Relative Humidity	10 – 95%, non-condensing
Atmospheric pressure	50 –106 kPa
Storage conditions	Corrosive-free and ventilated indoors
<b>AC Power Supply</b>	
Voltage	100 - 240 V~
Frequency	50/60 Hz
Current	0.40-0.14A
Fuse	Low interrupting rating, T5AL/250V
<b>External DC power supply</b>	
Voltage	DC 10V-16V
Current	2.25-1.5A

## A.2 Physical Specifications

Components	Weight	Size	Remark
Host	Less than 1.8 kg (Without pole clamp)	Less than 150 x 90 x 200 (mm) (length × width × height) (Without pole clamp)	Battery included

---

## A.3 Hardware Specifications

### A.3.1 Display

Display	
Type	Monochrome LCD
Size (diagonal)	2.5 inches
Differentiation	132 x 32 pixels

### A.3.2 Battery

Internal battery	
No. of batteries	1 (standard) or 2 (optional)
Battery type	Lithium battery
Shutdown delay	At least 30 mins (new battery, after the first low battery alarm)
Rated battery voltage	7.4 VDC
Battery capacity	2600 mAh (1 battery) or 5200 mAh (2 batteries)
Power supply time	Continuously operate at a rate of 25 ml/h, disable Wi-Fi function, discharge for at least 4h (1 battery) or 8h (2 batteries) using a fully charged new battery. Continuously operate at the maximum selectable rate, disable Wi-Fi function, discharge for at least 2h (1 battery) or 4h (2 batteries) using a fully charged new battery.
Charging time	When the pump is off, the charging time is not longer than 6h (1 battery) or 12h (2 batteries).

### A.3.3 Host LED

Host LED	
Alarm light	1 (two colors: red and yellow)
AC/DC indicator light	1 (green)
Batterys indicator light	1 (green)

### A.3.4 Auditory Indicator

Speaker	Produce an alarm, the sound pressure is 55 - 80 dB(A) and key beep; Support multi-level volume functions; The alarm sound meets the requirements of the IEC60601-1-8 standard.
---------	--

### A.3.5 External Ports

Ports	
AC power supply port	1 AC power supply port
DB9 interface	1 DB9 interface, which combines the following interface functions: <ul style="list-style-type: none"> <li>■ DC power input interface</li> <li>■ RS232 interface</li> <li>■ Nurse call interface</li> </ul>
Drop sensor interface	1 Drop sensor interface

### A.3.6 Signal Output Interface

Nurse call signal output	
Driving mode	Relay drive
Electric specification	C C
Isolation voltage	>1500 VAC
Action mode	Normally open or normally closed (optional)

## A.4 Wi-Fi Specifications

Protocol	IEEE 802.11b/g/n
Modulation mode	CCK and OFDM
Operating frequency	2412~2484MHz
Channel spacing	5MHz
Data rate	IEEE 802.11b: 1 - 11 Mbps IEEE 802.11g: 6 - 54 Mbps IEEE 802.11n: 6.5 - 150 Mbps
Transfer power	802.11b: +18dBm(Max) 802.11g: +16dBm(Max) 802.11n: +15dBm(Max)
Operating mode	STA/AP/STA+AP
Data security	WEP/WPA-PSK/WPA2-PSK

## A.5 Specifications

Parameters	Specifications
Infusion set standard	Infusion set used in conjunction with veterinary infusion pump should meet the requirements of ISO 8536-4:2004 Infusion equipment for medical use— Part 4: Infusion sets for single use, gravity feed, MOD
Compatible infusion set sizes (ml)	Infusion set diameter: 3.5-4.5mm Infusion set thickness: 0.8-1.2mm
Rate range	<ul style="list-style-type: none"> <li>■ Unit of Rate (ml/h): 0.1-1500, the increment is 0.1 ml/h</li> <li>■ Unit of Rate (drop/min): 1-(400 ml/h *drip/60), the increment is 1 drop/min</li> </ul>
Drip range	10-60 drop/ml, the increment is 1 drop/ml
Bolus rate range	0.1-1500ml/h Note: Bolus accuracy is not declared.
Purge rate range	600ml/h, nonadjustable
VTBI range	0.1-9999 ml, the increment is 0.1 ml
Volume range	0.1-9999 ml, the increment is 0.1 ml
Time display range	00:00:01-99:59:59 h:m:s



---

## A.6 A Reference Table Showing Occlusion Alarm

### Delay and Possible Dose

Occlusion pressure (Level)	Rate (ml/h)	Time of occlusion alarm (hh:mm:ss)	Bolus (ml)
Low	0.1	01:16:46	0.040
	1	00:07:25	0.033
	25	00:00:08	0.021
Medium	1	00:25:57	0.050
	25	00:00:48	0.028
High	0.1	08:36:34	0.069
	1	00:44:08	0.055
	25	00:01:45	0.037

#### NOTE

---

- **Test conditions:**

FLUKE IDA4 PLUS tester

Infusion set brand: SK

Test temperature: 20±2°C

Extension tube length: 1 meter

- **Occlusion alarm pressure, alarm delays and bolus volume may vary depending on test conditions, temperature and tube length.**
  - **The above data are only typical values under normal test conditions. The actual data may vary as test conditions change. Please refer to the test data for the product you have purchased. Under the same standard occlusion value and rate, the higher the value of the tested pressure is, the longer the alarm time will be delayed.**
-

---

## A.7 Infusion Accuracy Curve and Trumpet Curve

The following typical infusion accuracy table expresses performance after infusion has started and infusion fluctuations occurring within a certain period of time after normal infusion flow volumes have been reached. The infusion accuracy table is for reference only, detailed infusion accuracy curve is in accordance with the final device.

Plotted on the basis of data collected over a two-hour measurement period.

Infusion set brand: SK

Sampling quantity of pump: 3

Sampling quantity of infusion set: 3

Sampling interval:  $\Delta t = 0.5$  min

Test period:  $t = 240$  mins

Infusion rate:  $Q$  (m/h)

Flow rate deviation over time ( $p\Delta t$ )

Sampling interval:  $\Delta t = 0.5$  min

Observation windows:  $p\Delta t = 1, 2, 5, 11, 19, 31$  mins

Maximum deviation over the course of a full observation window:  $Ep(\text{Max})$  (%)



Minimum deviation over the course of a full observation window:  $Ep(\text{Min})$  (%)





Average deviation:  $A$  (%) and  $B$  (%)

### NOTE

- 
- Infusion accuracy may be influenced by the pump's environment (such as pressure, temperature, humidity and any infusion consumables used).
- 


- Unit of Rate (ml/h)

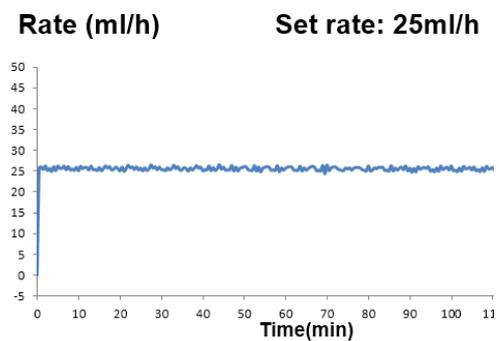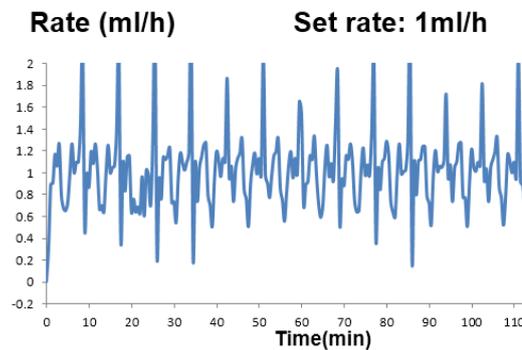

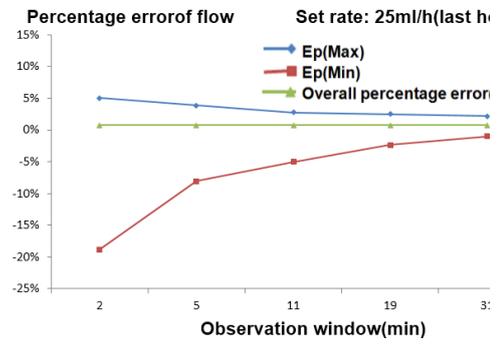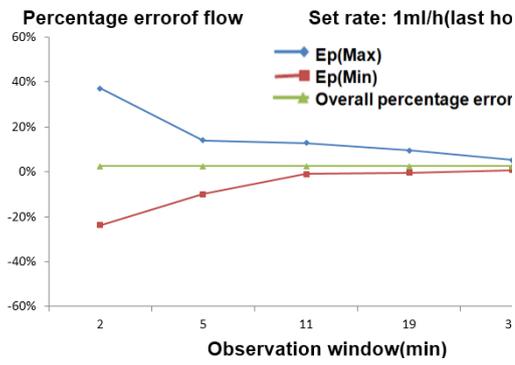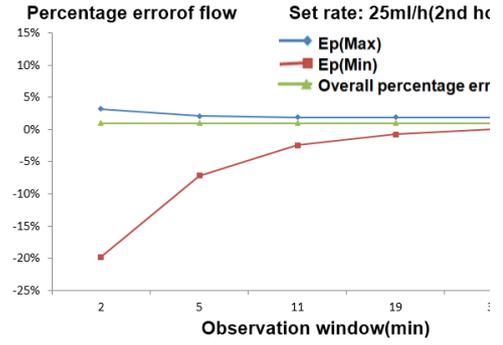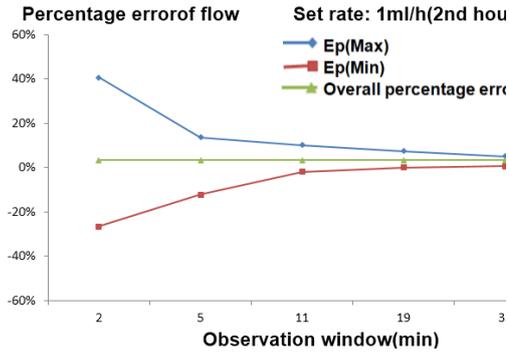


■ Unit of Rate (Drop/min)


Sampling rate: 20 Drop/min  
 Sampling interval:  $\Delta t = 1$  min  
 Test period:  $t = 120$  mins  
 Infusion rate:  $Q$  (Drop/min)

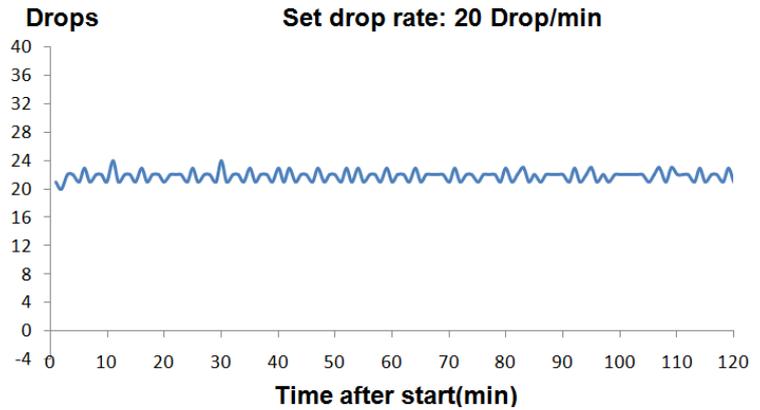

Sampling rate: 20 Drop/min  
 Sampling interval:  $\Delta t = 1$  min  
 Observation windows:  $p\Delta t = 1, 2, 5, 11, 19, 31$  mins  
 Maximum deviation over the course of a full observation window:  $Ep(\text{Max})$  (%)  
 Minimum deviation over the course of a full observation window:  $Ep(\text{Min})$  (%)  
 Average deviation:  $A$  (%)

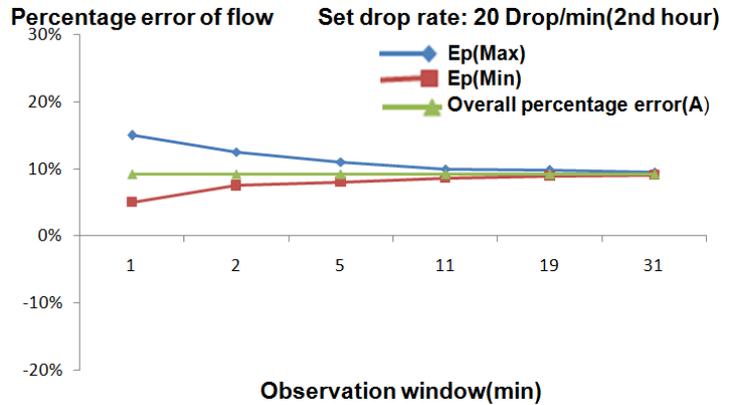

Sampling rate: 20 Drop/min  
 Sampling interval:  $\Delta t = 1$  min  
 Observation windows:  $p\Delta t = 1, 2, 5, 11, 19, 31$  mins  
 Maximum deviation over the course of a full observation window:  $Ep(\text{Max})$  (%)  
 Minimum deviation over the course of a full observation window:  $Ep(\text{Min})$  (%)  
 Average deviation:  $B$  (%)

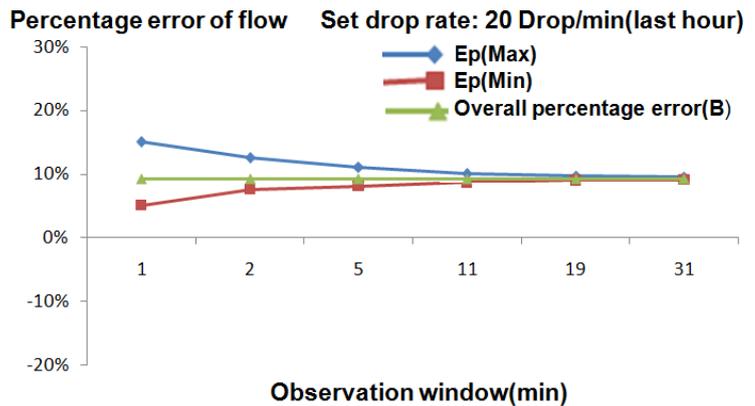

# **B** EMC and Radio Regulatory Compliance

---

---

## **B.1 EMC**

The device meets the requirements of IEC 60601-1-2:2014.

### **NOTE**

---

- **Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this device could result in increased electromagnetic emissions or decreased electromagnetic immunity of this device and result in improper operation.**
  - **Use of this device adjacent to or stacked with other device should be avoided because it could result in improper operation. If such use is necessary, this device and the other device should be observed to verify that they are operating normally.**
  - **Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the this device, including cables specified by the manufacturer. Otherwise, degradation of the performance of this device could result.**
  - **The non-ME EQUIPMENT (e.g. ITE) that is a part of an ME SYSTEM may be disrupted by the electromagnetic interference of nearby equipment. It may be necessary to take mitigation measures, such as re-orienting or relocating the non-ME EQUIPMENT or shielding the location.**
  - **This device is intended for use in professional healthcare facility environment only. If it is used in special environment, such as magnetic resonance imaging environment, the equipment/system may be disrupted by the operation of nearby equipment.**
-

<b>Guidance and Declaration - Electromagnetic Emissions</b>		
The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.		
<b>Emission test</b>	<b>Compliance</b>	<b>Electromagnetic environment - guidance</b>
Conducted and radiated RF EMISSIONS CISPR 11	Group 1	The device uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic device.
Conducted and radiated RF EMISSIONS CISPR 11	Class A	The device is suitable for use in all establishments other than domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic distortion IEC 61000-3-2	Class A	The device is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Voltage fluctuations and flicker IEC 61000-3-3	Complies	

## **NOTE**

- **The device needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided below.**
- **Other devices may affect this device even though they meet the requirements of CISPR.**
- **The EMISSIONS characteristics of this device make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this device might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as relocating or re-orienting the device.**
- **If the essential performance is lost or degraded, it may be necessary to take mitigation measures, such as re-orienting or relocating the ME EQUIPMENT or ME SYSTEM or shielding the location or stopping using the veterinary infusion pump system and contact the service personnel.**

If the device is operated within the electromagnetic environment listed in Table **Guidance and Declaration —Electromagnetic Immunity**, the system will remain safe and provide the following essential performance:

- Operating mode
- Accuracy
- Function
- Protection against UNINTENDED BOLUS volumes
- Occlusion
- ALARM CONDITIONS regarded
- Data stored

<b>Guidance and Declaration - Electromagnetic Immunity</b>			
The device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.			
<b>Immunity test</b>	<b>IEC 60601 test level</b>	<b>Compliance level</b>	<b>Electromagnetic environment - guidance</b>
Electrostatic discharge (ESD) IEC 61000-4-2	±8 kV contact ±15kV air	±8 kV contact ±15kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines (length greater than 3 m)	±2 kV for power supply lines ±1 kV for input/output lines (length greater than 3 m)	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV line(s) to line(s) ±2 kV line(s) to earth	±1 kV line(s) to line(s) ±2 kV line(s) to earth	
Voltage dips and Voltage interruptions IEC 61000-4-11	0 % $U_T$ for 0,5 cycle  0 % $U_T$ for 1 cycle and 70 % $U_T$ for 25/30 cycles	0 % $U_T$ for 0,5 cycle  0 % $U_T$ for 1 cycle and 70 % $U_T$ for 25/30 cycles	Mains power quality should be that of a typical commercial or hospital environment. If the user of our product requires continued

	0 % U <sub>T</sub> for 250/300 cycle	0 % U <sub>T</sub> for 250/300 cycle	operation during power mains interruptions, it is recommended that our product be powered from an uninterruptible power supply or a battery.
RATED power frequency magnetic fields IEC 61000-4-8	30 A/m 50 Hz / 60 Hz	30 A/m 50 Hz / 60 Hz	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
Note: U <sub>T</sub> is the A.C. mains voltage prior to application of the test level.			

<b>Guidance and Declaration - Electromagnetic Immunity</b>			
The device is intended for use in the specified electromagnetic environment. The customer or the user of the device should assure that it is used in such an environment as described below.			
<b>Immunity test</b>	<b>IEC 60601 Test level</b>	<b>Compliance level</b>	<b>Electromagnetic environment - guidance</b>
Conducted disturbances induced by RF fields IEC61000-4-6	3 Vrms 150 kHz to 80 MHz	10 Vrms	Portable and mobile RF communications equipment should be used no closer to any part of the device, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance: $d = \left[ \frac{3.5}{V} \right] \sqrt{P}$ 150k to 80 MHz
	6 Vrms in ISM bands and amateur radio bands <sup>a</sup> between 0,15 MHz and 80 MHz	6 Vrms	
Radiated RF EM fields IEC61000-4-3	10V/m 80 MHz to 2.7 GHz	10V/m	$d = \left[ \frac{3.5}{E} \right] \sqrt{P}$ 80 MHz to 800 MHz $d = \left[ \frac{7}{E} \right] \sqrt{P}$ 800 MHz to 2.7 GHz
Proximity fields from RF	27 V/m 380–390 MHz	27 V/m	where P is the maximum output power rating of the transmitter in watts (W) according to the

wireless communication equipment IEC61000-4-3	28 V/m 430–470 MHz, 800–960 MHz, 1700–1990 MHz, 2400–2570 MHz	28 V/m	transmitter manufacturer and d is the recommended separation distance in meters (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey <sup>b</sup> , should be less than the compliance level in each frequency range <sup>c</sup> . Interference may occur in the vicinity of equipment marked with the following symbol:  .
	9 V/m 704–787 MHz, 5100–5800 MHz	9 V/m	

Note 1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

<sup>a</sup> The ISM (industrial, scientific, and medical) bands between 150 kHz and 80 MHz are 6.765 MHz to 6.795 MHz; 13.553 MHz to 13.567 MHz; 26.957 MHz to 27.283 MHz; and 40.66 MHz to 40.70 MHz. The amateur radio bands between 0,15 MHz and 80 MHz are 1,8 MHz to 2,0 MHz, 3,5 MHz to 4,0 MHz, 5,3 MHz to 5,4 MHz, 7 MHz to 7,3 MHz, 10,1 MHz to 10,15 MHz, 14 MHz to 14,2 MHz, 18,07 MHz to 18,17 MHz, 21,0 MHz to 21,4 MHz, 24,89 MHz to 24,99 MHz, 28,0 MHz to 29,7 MHz and 50,0 MHz to 54,0 MHz.

<sup>b</sup> Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the device is used exceeds the applicable RF compliance level above, the device should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the device.

<sup>c</sup> Over the frequency ranges 150 kHz to 80 MHz, field strengths should be less than 3V/m.

**Recommended Separation Distances between Portable and Mobile RF, Communications Equipment and This Equipment**

The equipment is intended for use in an electromagnetic environment in which radiated RF disturbance are controlled. The customer or the user of the device can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the device as recommended below, according to the maximum output power of the communication equipment.

Rated Maximum Output power of Transmitter Watts (W)	Separation Distance According to Frequency of Transmitter (m)		
	150 kHz to 80 MHz $d = \left[ \frac{3.5}{V} \right] \sqrt{P}$	80 MHz to 800 MHz $d = \left[ \frac{3.5}{E} \right] \sqrt{P}$	800 MHz to 2.7 GHz $d = \left[ \frac{7}{E} \right] \sqrt{P}$
0.01	0.04	0.04	0.07
0.1	0.11	0.11	0.22
1	0.4	0.4	0.7
10	1.1	1.1	2.2
100	4	4	7

For transmitters at a maximum output power not listed above, the recommended separation distanced in meters (m) can be determined using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

Note 1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

## B.2 Radio Regulatory Compliance

RF Parameter

Radio devices	IEEE 802.11b/g/n (2.4GHz Wi-Fi)
Operating frequency	2412MHz to 2484MHz
Modulation mode	CCK, OFDM
Output power	dBm



The radio device used in this product is in compliance with the essential requirements and other relevant provisions of Directive 2014/53/EU.

# C Default Factory Settings

---

---

This chapter presents some default factory settings. User cannot change the factory default, but may restore to the default factory settings when it is necessary.

## C.1 Alarms

Alarm Setting	Factory Default
Volume	4
Alarm sound	Sound2

## C.2 Interface

UI	Factory Default
Brightness	4

## C.3 Parameters

Setting Parameters	Factory Default
KVO rate	0.5ml/h
Pressure unit	mmHg
Occl. pressure	525mmHg
Bubble size	10 l
Accum. bubble	1.5ml/h
Auto-lock	Off
Empty Alarm	Low
Reminder	2min
Near end	3min
Commonly used tube	B. Braun, SK
Bed No.	---
Standby time range	24:00

---

## C.4 System Time

System Date and Time	Factory Default
Time	00:00
Date	01/01/2015

# D Alarm Information

This chapter presents the alarm information of the infusion pump. Prompt information for operation guidance will not be presented in this chapter.

The table shows the appropriate countermeasures for each piece of information related to alarm triggering. If the problem still exists after operating according to the countermeasures, please contact the company.

Alarm Information	Alarm level	Reason	Countermeasure
[Occlusion]	High	When occlusion occurs in the infusion tube between the device and the animal, and occlusion pressure reaches the threshold value.	Press  to cancel alarm, eliminate the causes of the pressure of infusion tube, and then press  to continue the infusion.
[Air in line]	High	Size of single bubble or bubbles accumulated in 1 hour reaches to the preset value.	Press  to cancel alarm.
[Door opened]	High	The veterinary infusion pump door is opened during infusion.	Press  to cancel alarm and close the door correctly.
[VTBI Done]	High	VTBI volume is completed.	Press  to cancel alarm.
[KVO Finish]	High	Alarm is triggered when KVO model runs 30 minutes.	Press  to cancel alarm.
[Battery Low]	Low	Only powered with built-in battery, battery charge is insufficient.	Connect to the power source to cancel alarm automatically.
[Battery Empty]	High	Only powered with built-in battery, battery is empty.	Connect to the AC power source, press  or  to cancel alarm.
[AC Power Disconnection]	Low	Power cord disconnected when the network power	Connect to the power source to cancel alarm

Alarm Information	Alarm level	Reason	Countermeasure
		source supply is powered.	automatically.
[Reminder]	Low	The veterinary infusion pump performs no operation during the set reminder time after the infusion set is loaded to it.	Operate the pump or open the door to cancel alarm.
[System Error]	High	Motor operation error, data communication error, sensor failure and etc.	Alarm cannot be cancelled. Please stop operation and contact the company.
[VTBI Done] Near	Low	Required time for the remaining VTBI volume almost reaches the set [Near end].	1. The alarm will not be cancelled automatically until the infusion is completed, and then switch to [VTBI Done] alarm. 2. Or press  to cancel alarm.
[Standby Time Expired]	Mid-level	Standby is completed.	Press  to cancel alarm, and then exit standby or continue standby by pressing  .
[System abnormal]	Mid-level	Charging circuit error, supplying circuit error and etc.	Alarm cannot be cancelled. Please stop operation and contact the company.
[Tube not inserted]	Low	Door is opened during infusion, or infusion set is not loaded, and start infusion when the door is closed.	Correctly load infusion set and close the door.

Alarm Information	Alarm level	Reason	Countermeasure
[Drop error]	High	If drop sensor is installed correctly and the switch of [Drip rate check] is on, current rate is ml/h, drop sensor detects that the drop rate deviates the preset value.	Press  to cancel alarm.
[Empty bottle]	High	If drop sensor is installed correctly and the switch of [Drop sensor] is on, no liquid drop. Note: If drop sensor is not correctly inserted or the surface of the liquid in the drip chamber is abnormal, [Empty bottle] alarm might be triggered.	Press  to cancel alarm.
[No communication]	Low	Veterinary infusion pump and BeneFusion CS5 Infusion Supervision System are communicated successfully over Wi-Fi, the network communication is abnormally interrupted for 3 minutes. After the alarm is triggered, infusion of the pump will not be influenced, and the pump continues infusion.	Press  or restore the communication between veterinary infusion pump(s) and BeneFusion CS5 Infusion Supervision System.

## NOTE

- All alarm sounds can be paused by pressing , except for the circumstance of [Battery Empty].

---

FOR YOUR NOTES

# E Symbols and Terms

---

---

## E.1 List of Units

Abbreviation	Meaning
A	ampere
°C	centigrade
cm	centimeter
dB	decibel
g	gram
hr	hour
Hz	hertz
inch	inch
k	kilo
kg	kilogram
kPa	kilopascal
l	litre
lb	pound
m	meter
mg	milligrams
min	minute
ml	milliliter
mm	millimeters
mmHg	millimeters of mercury
s	second
	Microgram
V	volt
VA	volt ampere
W	watt

---

## E.2 List of Symbols

Symbols	Meaning
-	minus
%	percent
/	Per; divide; or
~	to
^	power
+	plus
=	equal to
<	less than
>	greater than
	less than or equal to
	greater than or equal to
±	plus or minus
×	multiply
©	copyright

## E.3 List of Terms

Abbreviation	Meaning
AC	Alternating current
Anti-Bolus	Anti-Bolus
BOLUS	Bolus
CCU(CICU)	Cardiac Intensive Care Unit
CE	Conformité Européenne
CISPR	International Special Committee on Radio Interference
CPU	central processing unit
DC	Direct current
DPS	Dynamic Pressure System
ECU(EICU)	Emergency Intensive Care Unit

<b>Abbreviation</b>	<b>Meaning</b>
EEC	European Economic Community
EMC	Electromagnetic compatibility
EMI	Electromagnetic interference
EtO	C2H4O
ICU	Intensive Care Unit
ID	Identification
IEC	International Electrotechnical Commission
IEEE	Institute of Electrical and Electronic Engineers
ISO	International organization for Standardization
KVO	Keep vein open
LED	light emitting diode
Max	Maximum
MDD	Medical Device Directive
Min	Minimum
MRI	magnetic resonance imaging
N/A	not applied
NICU	Newborn Intensive Care Unit
OR	operating room
SN	Series Number
TIVA	Total Intra Venous Anesthesia
VTBI	Volume To Be Infused

---

## E.4 List of Unit Conversion

Unit Symbols	Unit Conversion
kPa	1kPa=7.5mmHg=0.145psi=0.01bar
psi	1psi=51.724mmHg=6.897kPa=0.069bar
bar	1bar=750mmHg=14.5psi=100kPa
lb	1 lb=0.454kg
drop/min	drop/min = (ml/h×drip)/60

# F Toxic and Hazardous Substances or Elements

Name of the Parts		Pb	Hg	Cd	Cr(VI)	PBB	PBDE
		Pb	Hg	Cd	Cr(VI)	PBB	PBDE
Device housing	Front housing						
	Back housing						
	Keys						
	Facing						
	Labels						
Display	Display						
Host	Host hardware						
	Internal cables						
	PCBA						
Packaging	Cartons (K=K crimp paper)						
	Foam packages (EPE)						
	Plastic bag (PE)						
General	Connecting pieces						
	Power cord						
Battery	Battery						
Accessories	Accessories						
Remark	<p>: Indicates that this toxic or hazardous substance contained in all of the homogeneous materials for this part is below the limit requirement in Directive 2011/65/EU.</p> <p>×: Indicates that this toxic or hazardous substance contained in at least one of the homogeneous materials used for this part is above the limit requirement in Directive 2011/65/EU.</p>						

---

FOR YOUR NOTES



GERMANY

EICKEMEYER KG  
Eltastraße 8  
78532 Tuttlingen  
T +49 7461 96 580 0  
F +49 7461 96 580 90  
info@eickemeyer.de  
www.eickemeyer.de

SWITZERLAND

EICKEMEYER AG  
Sandgrube 29  
9050 Appenzell  
T +41 71 788 23 13  
F +41 71 788 23 14  
info@eickemeyer.ch  
www.eickemeyer.ch

POLAND

EICKEMEYER Sp. z o.o.  
Al. Jana Pawła II 27  
00-867 Warszawa  
T +48 22 185 55 76  
F +48 22 185 59 40  
info@eickemeyer.pl  
www.eickemeyer.pl

ITALY

EICKEMEYER S.R.L.  
Via G. Verdi 8  
65015 Montesilvano (PE)  
T +39 085 935 4078  
F +39 085 935 9471  
info@eickemeyer.it  
www.eickemeyer.it

DENMARK

EICKEMEYER ApS  
Solbakken 26, Hammelev  
6500 Vojens  
T +45 7020 5019  
info@eickemeyer.dk  
www.eickemeyer.dk

NETHERLANDS

EICKEMEYER B.V.  
Bellweg 44  
4104 BJ Culemborg  
T +31 345 58 9400  
info@eickemeyer.nl  
www.eickemeyer.nl

UNITED KINGDOM

EICKEMEYER Ltd.  
3 Windmill Business Village  
Brooklands Close  
Sunbury-on-Thames  
Surrey, TW16 7DY  
T +44 20 8891 2007  
info@eickemeyer.co.uk  
www.eickemeyer.co.uk

CANADA

EICKEMEYER Inc.  
617 Douro Street, Suite #205  
Stratford, Ont. Canada  
N5A 0B5  
T +1 519 273 5558  
F +1 519 271 7114  
info@eickemeyervet.ca  
www.eickemeyercanada.ca